

110



Fig. 12A

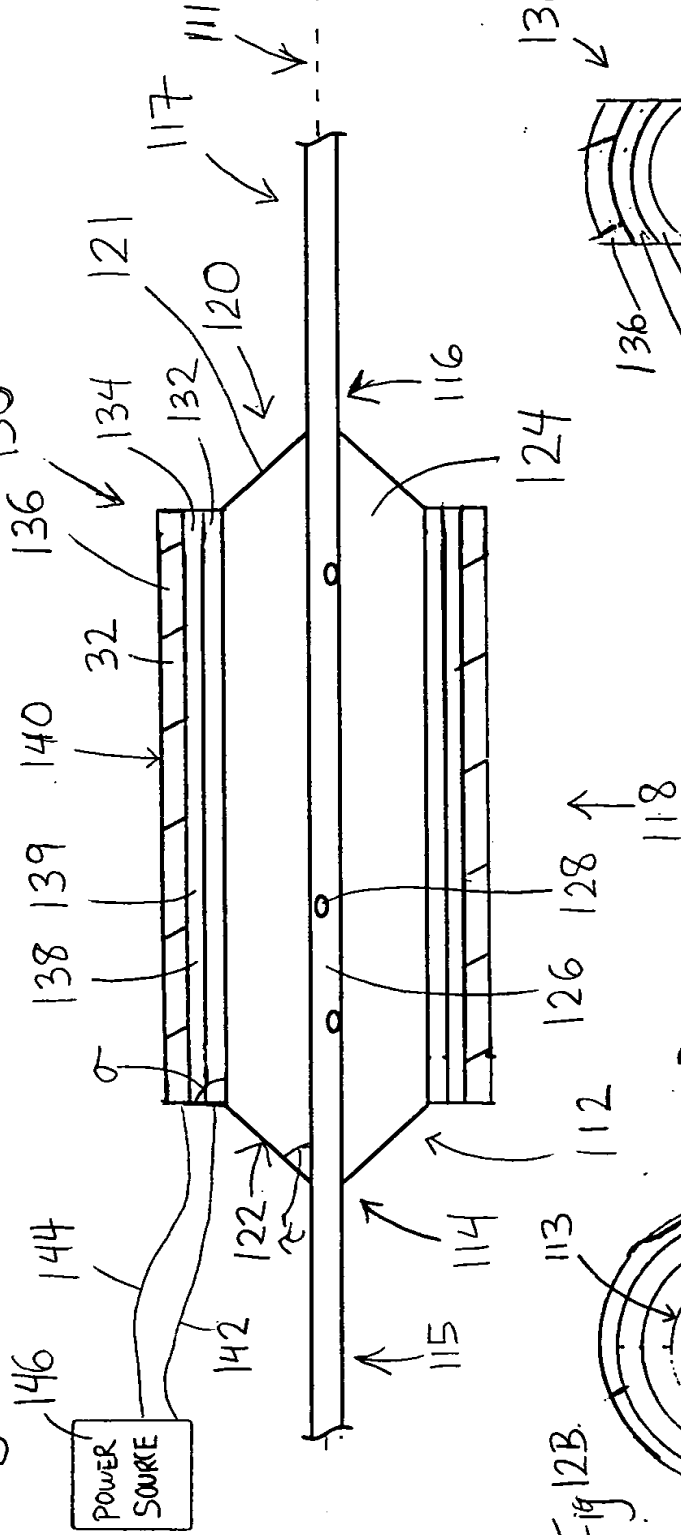


Fig. 12B

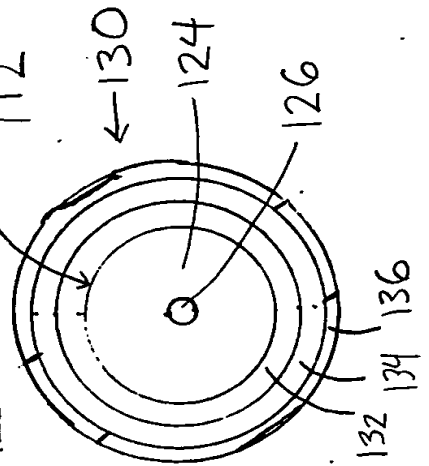
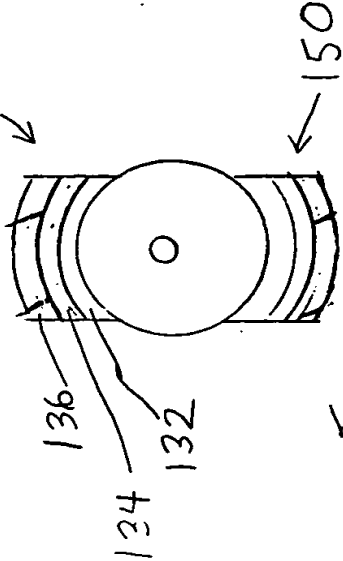
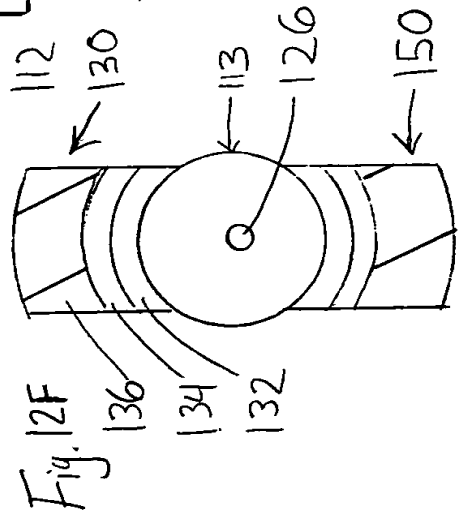
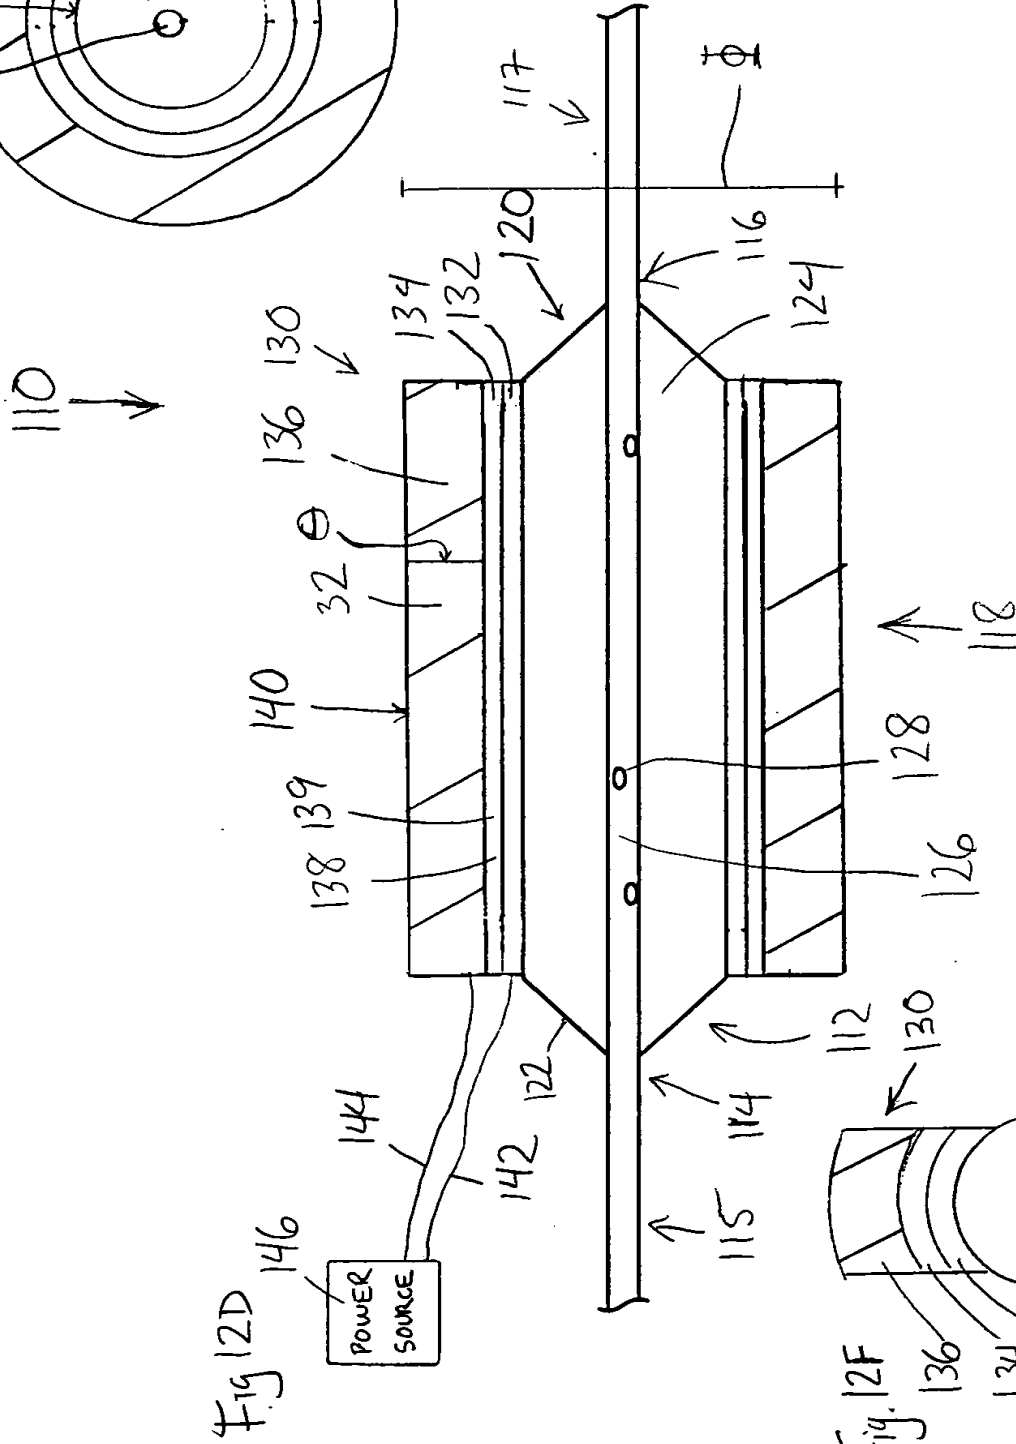
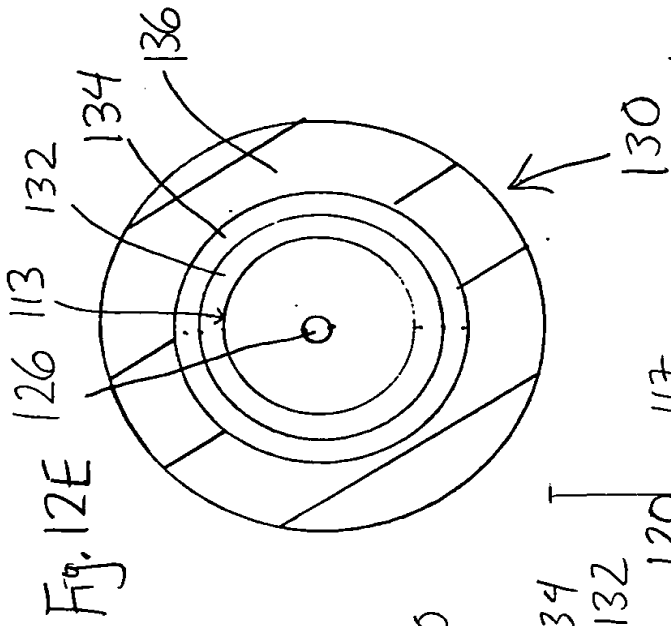


Fig. 12C





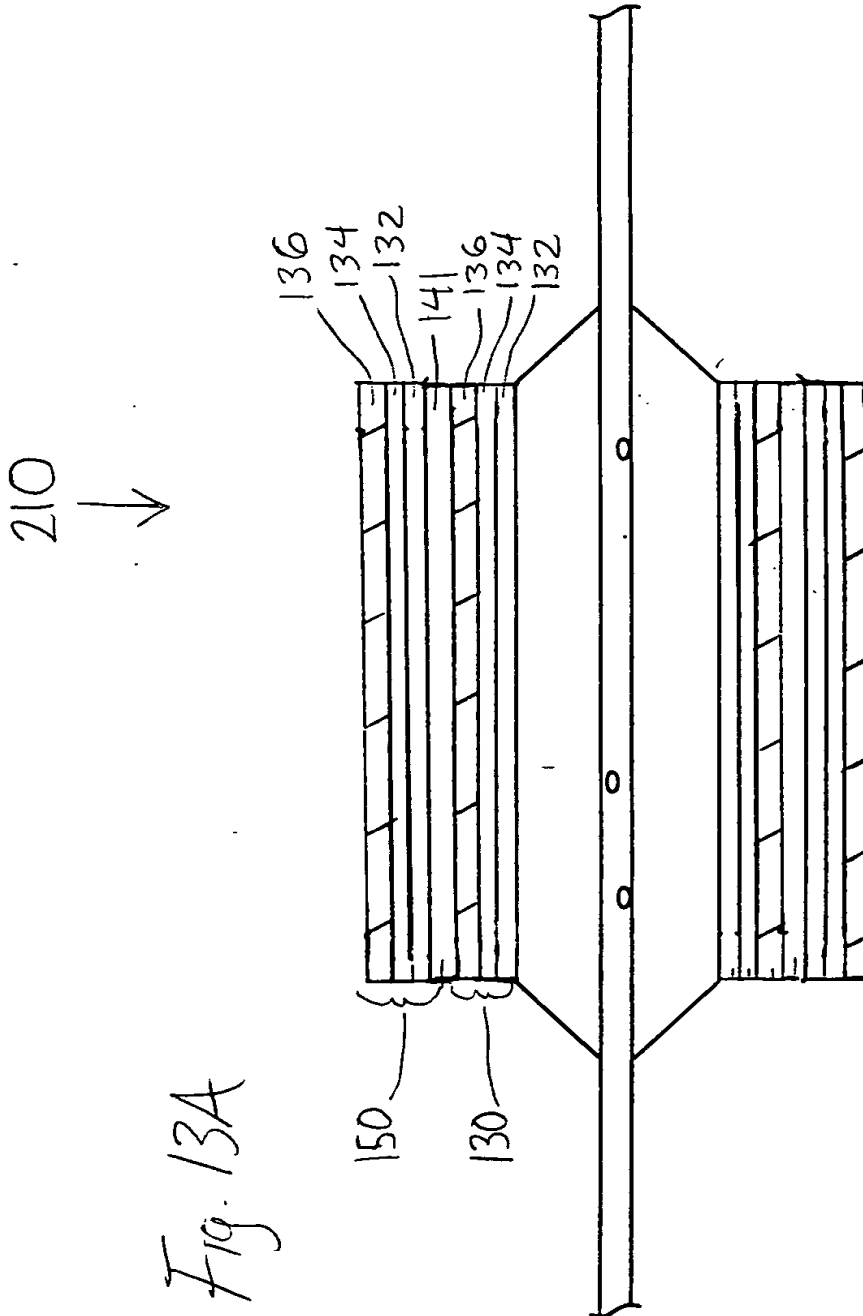
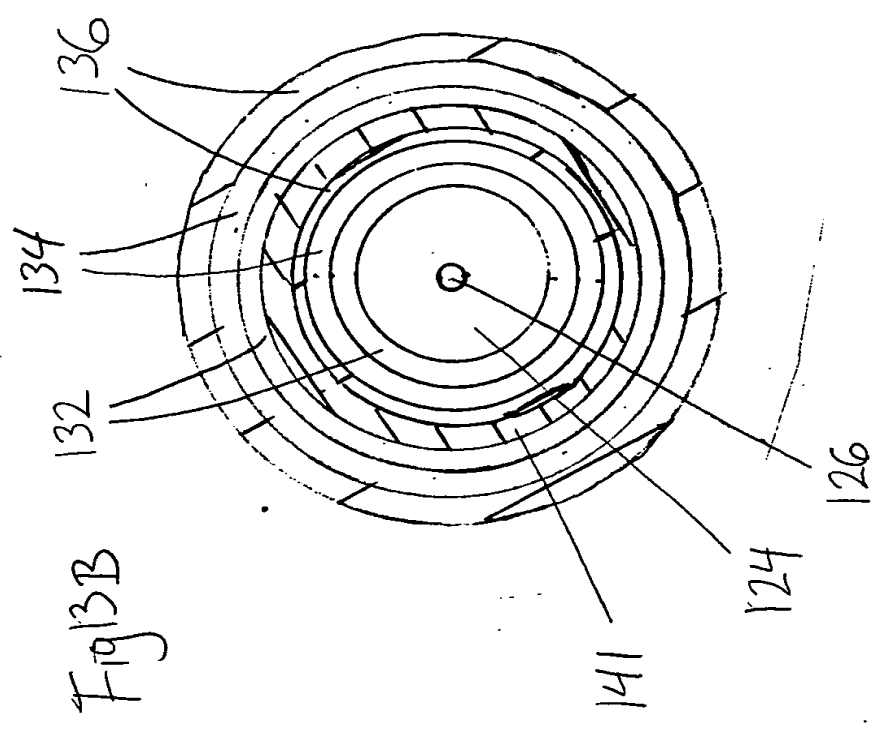
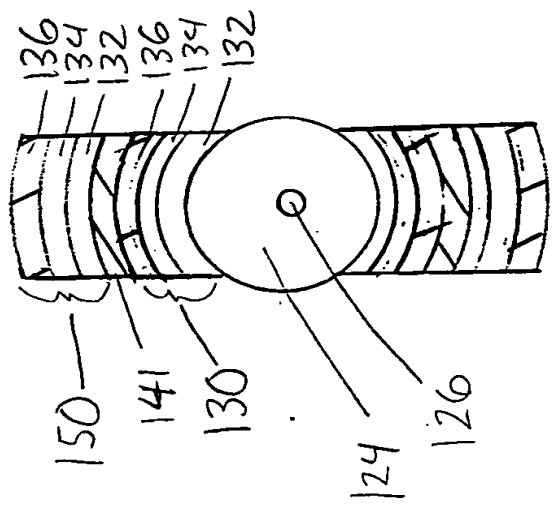


Fig. 13C






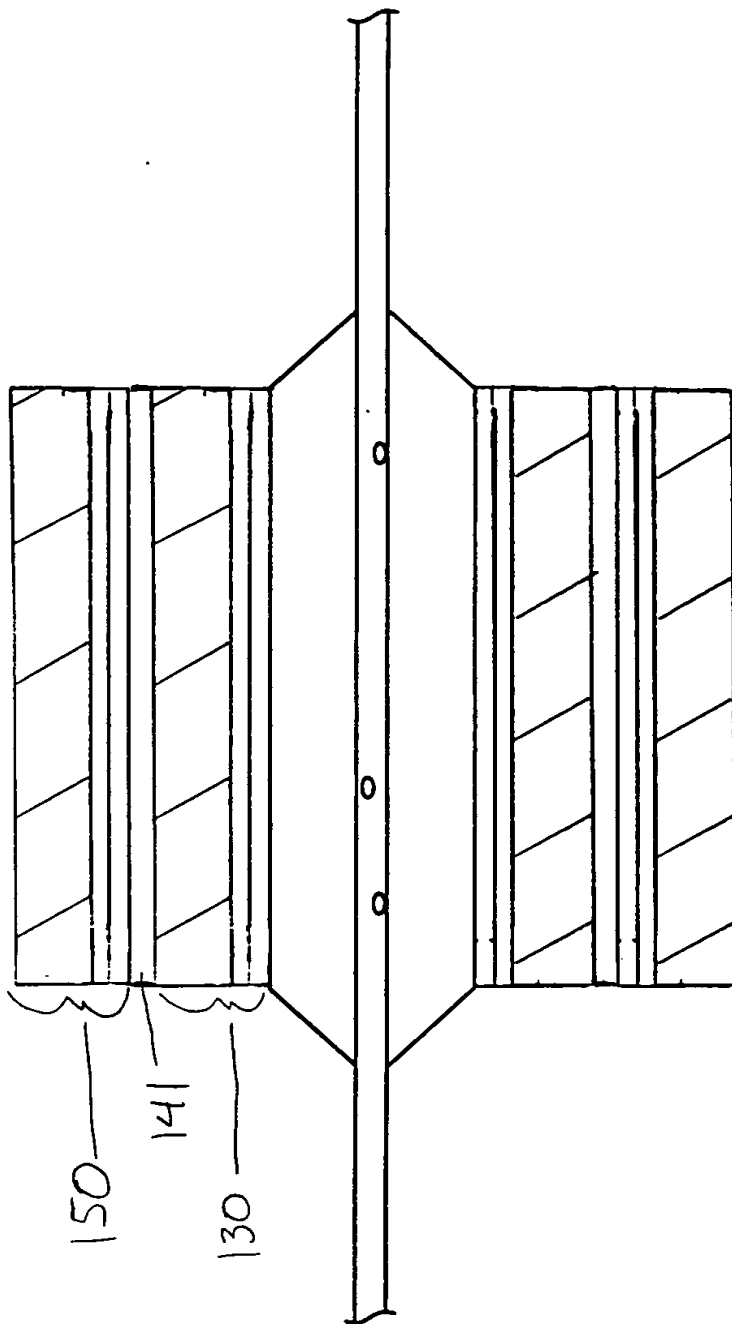


Fig. 13D

Fig 13F

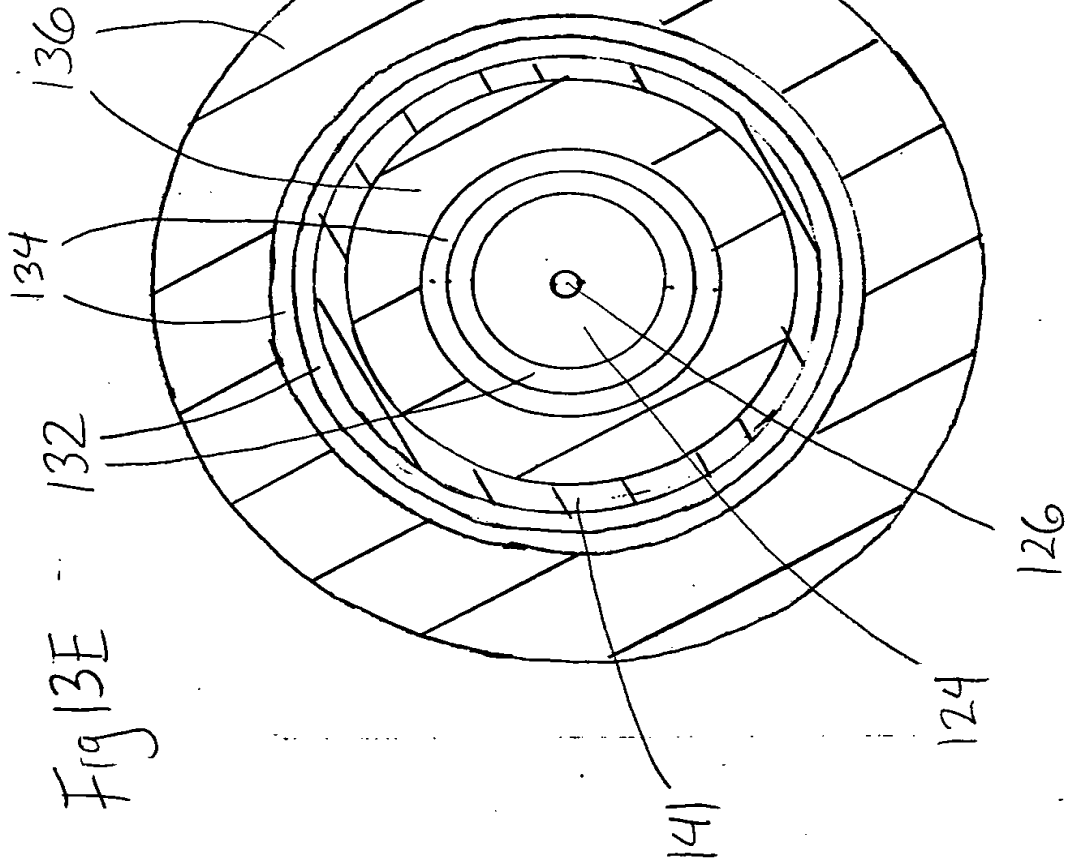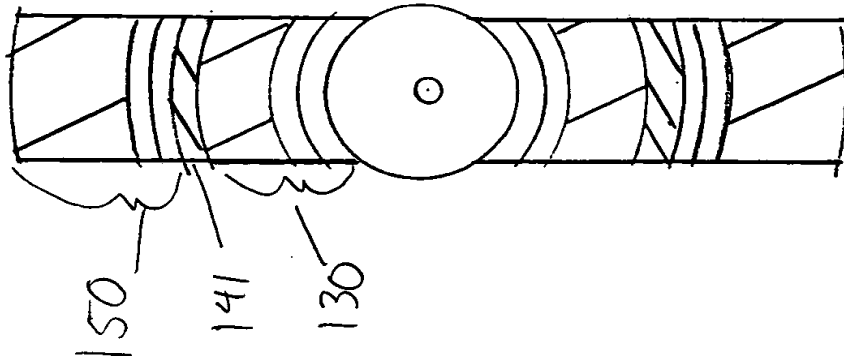

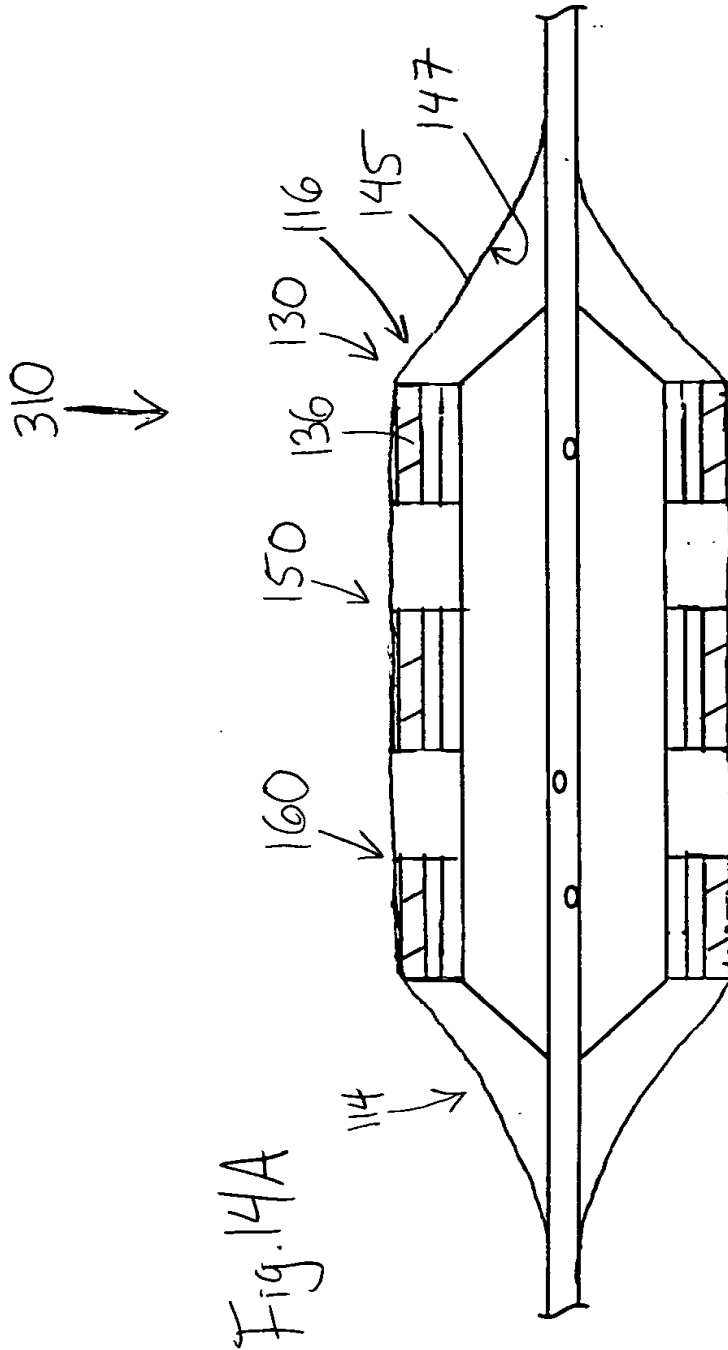

310
↓

136


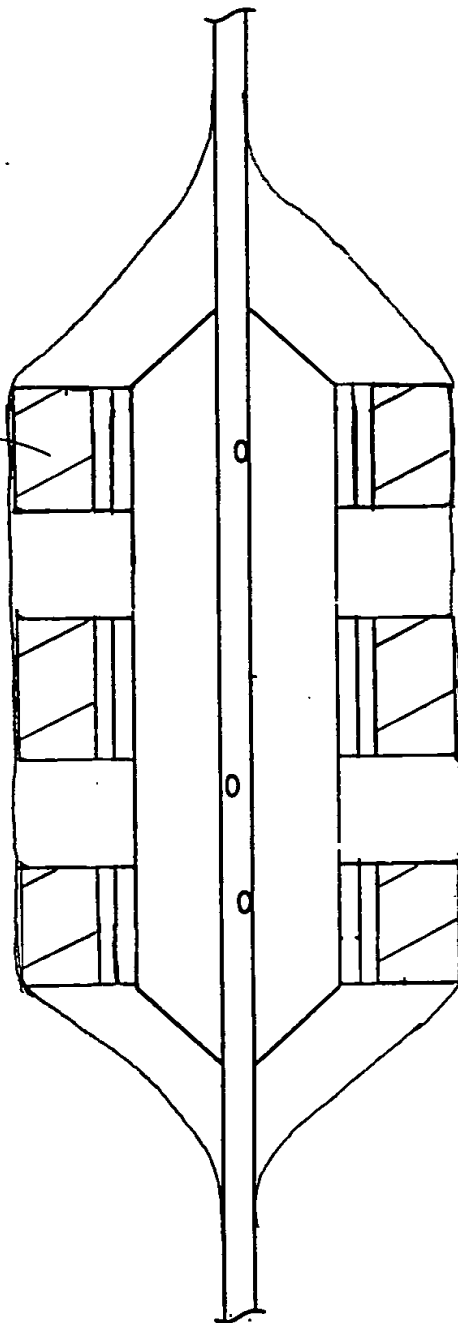


Fig. 14B


410
↓

Fig. 15A

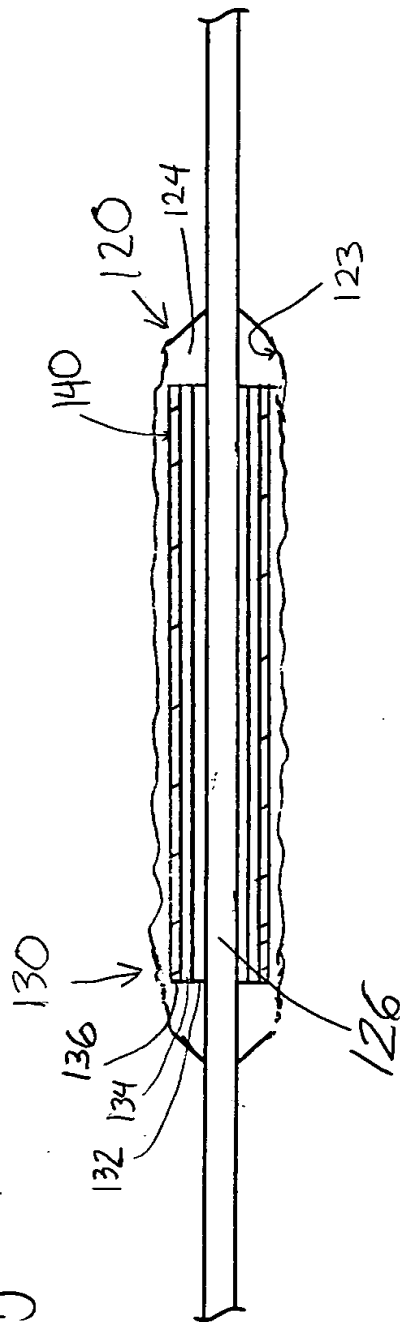

410
↓

Fig. 15B

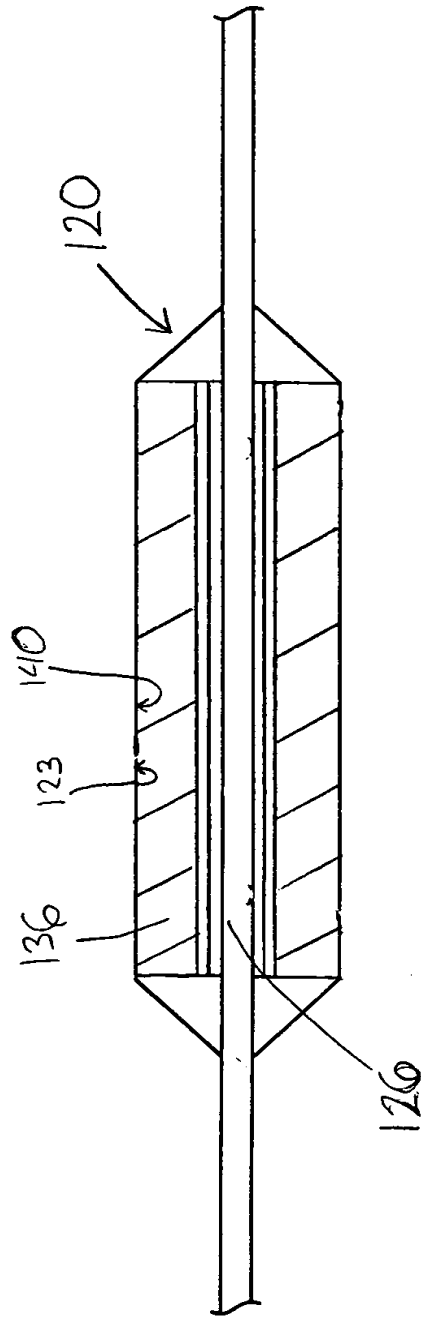

510
↓

130
136
126

Fig 16A



510
↓

130 136
126

Fig. 16B

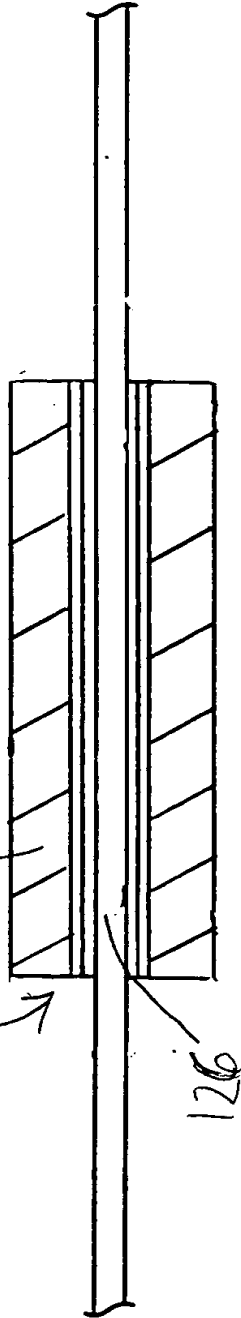
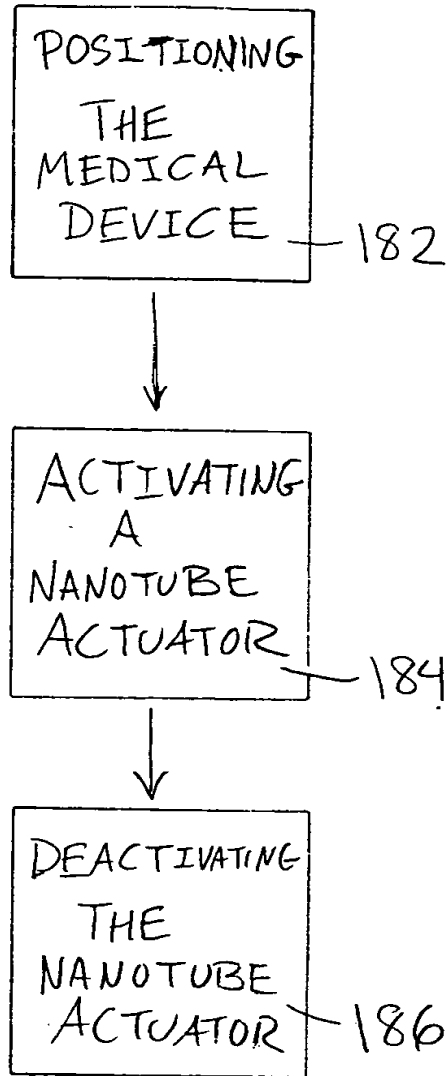


Fig: 17

180
↙



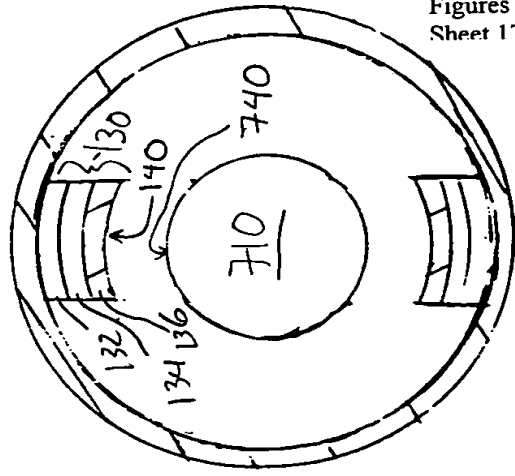


Fig 18B

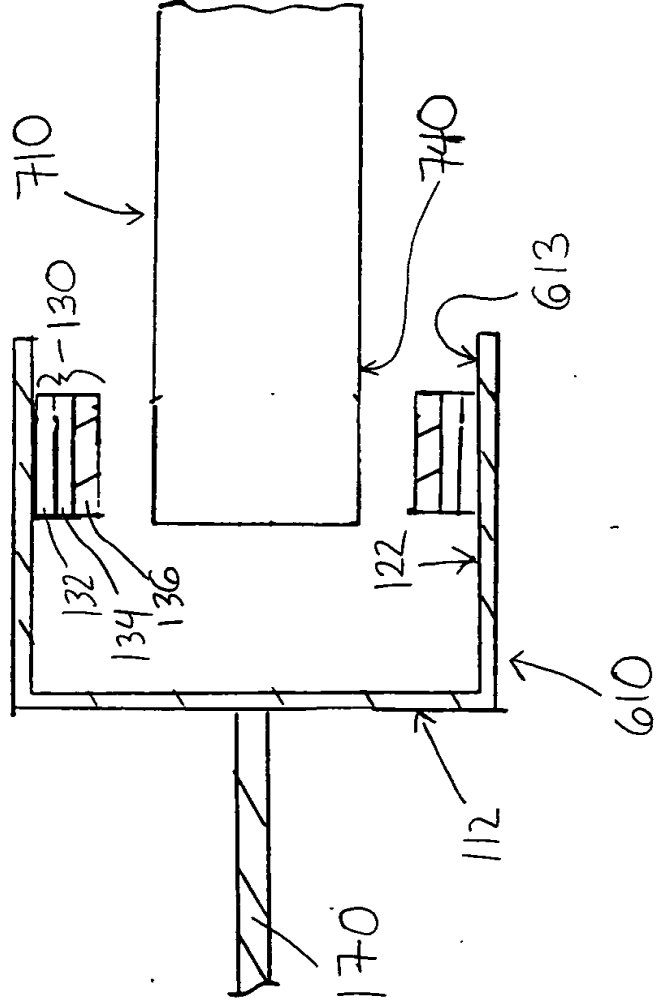


Fig 18A

Fig. 18D

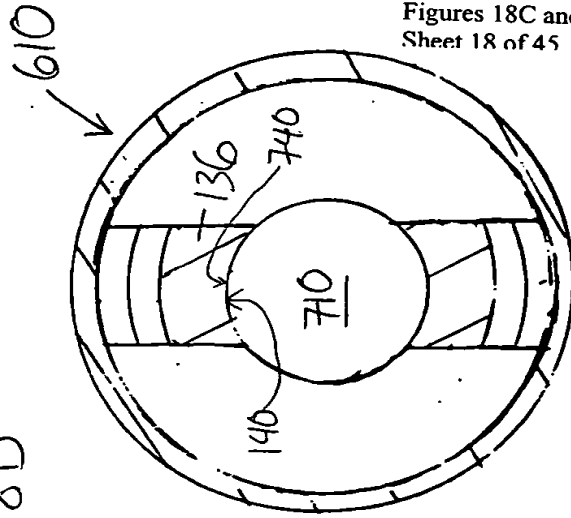


Fig 18C

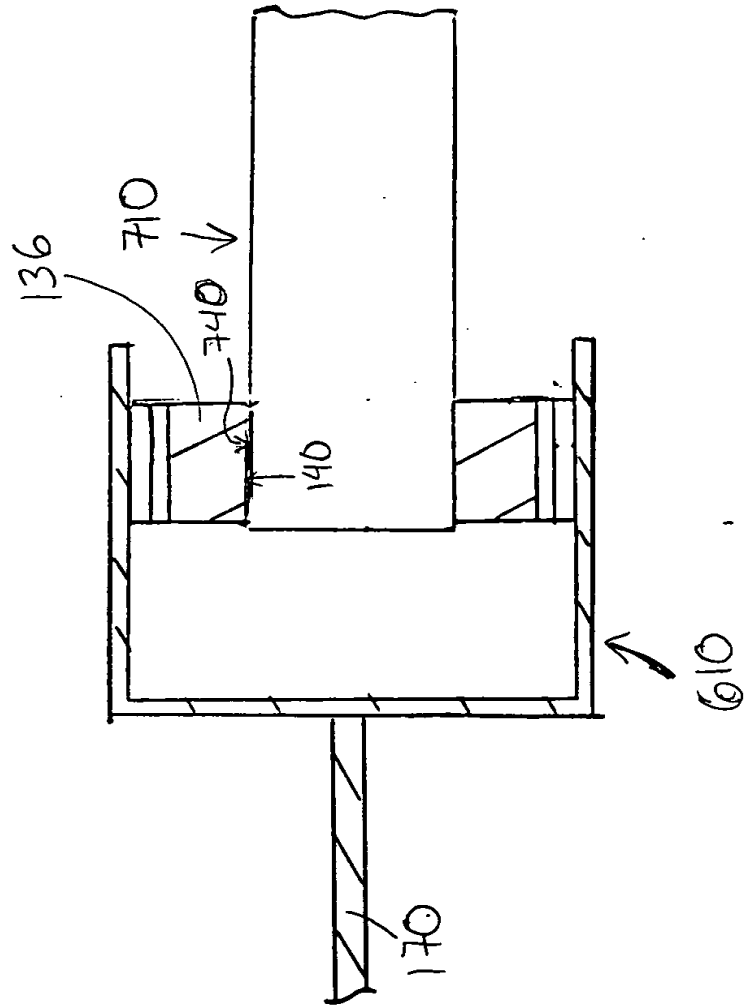


Fig 19A

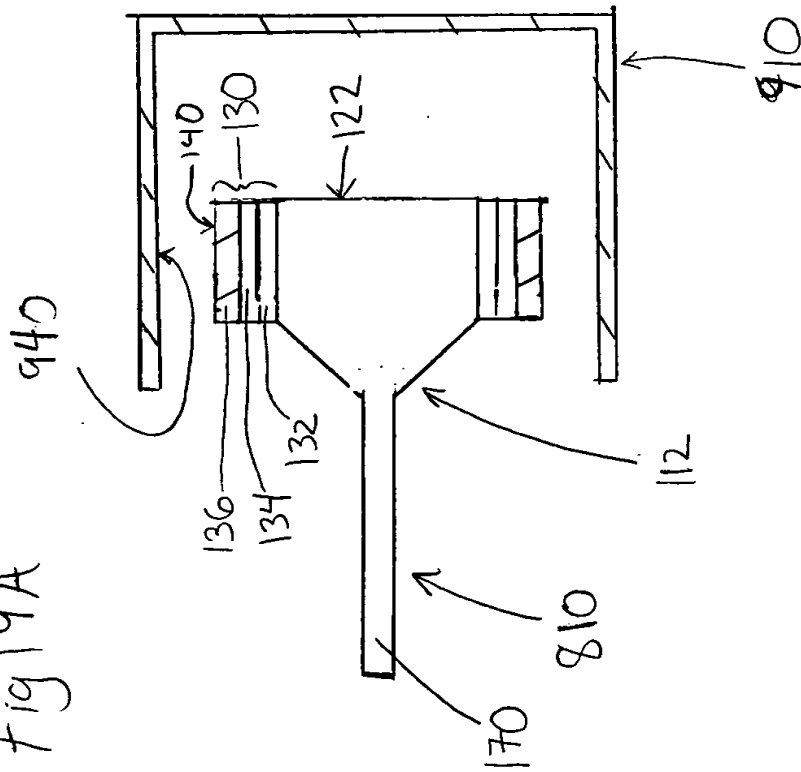
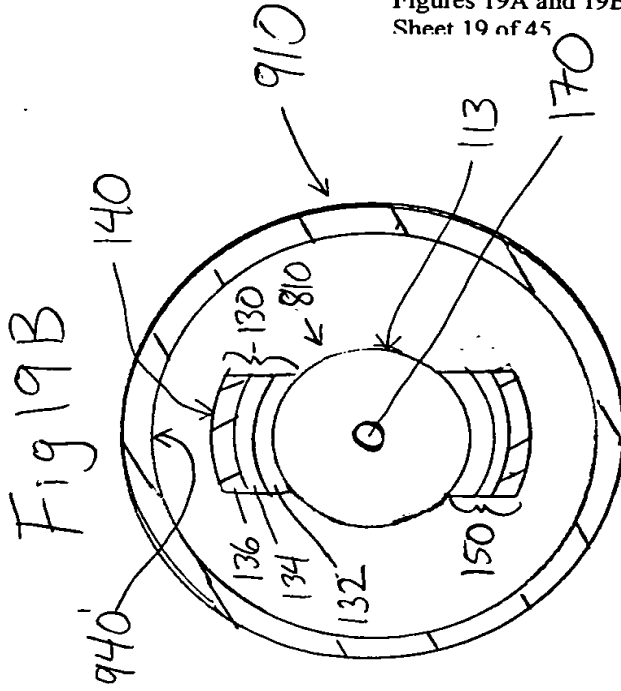


Fig 19B



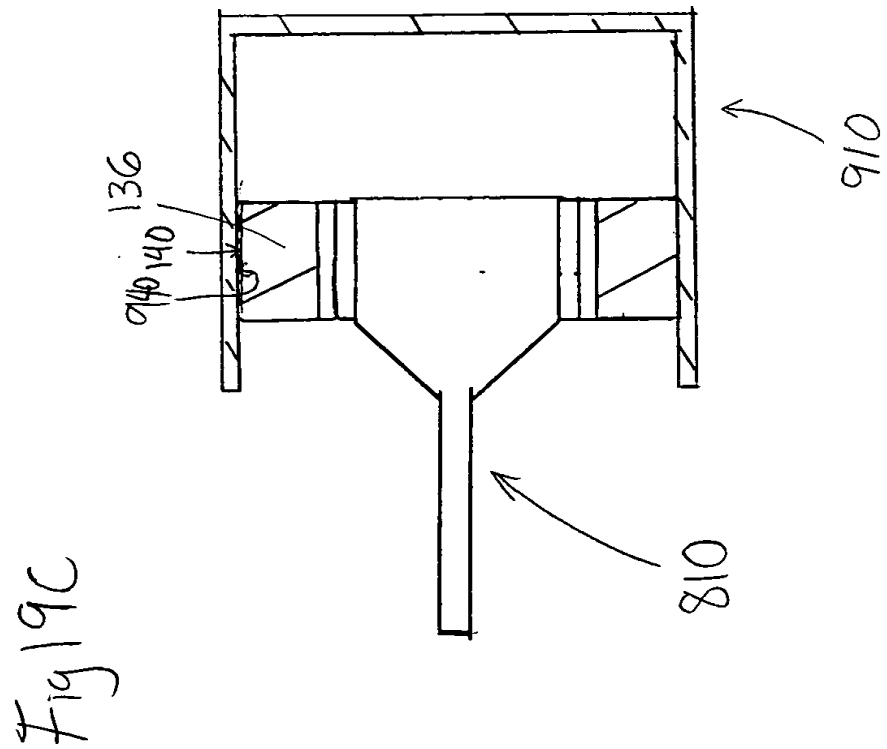
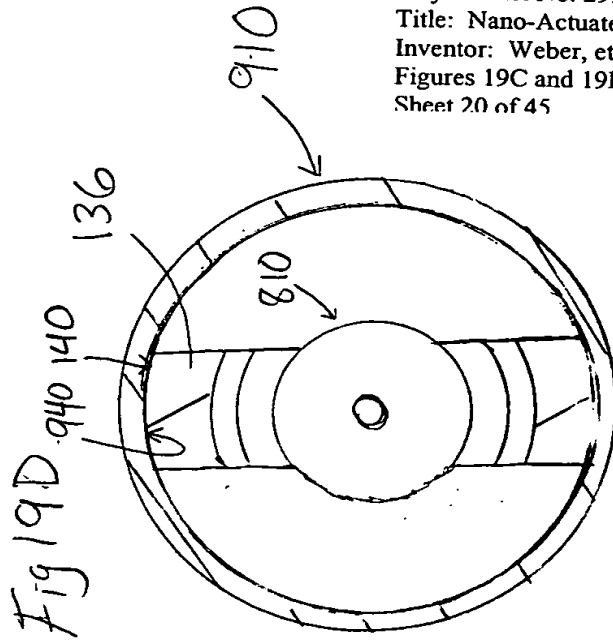
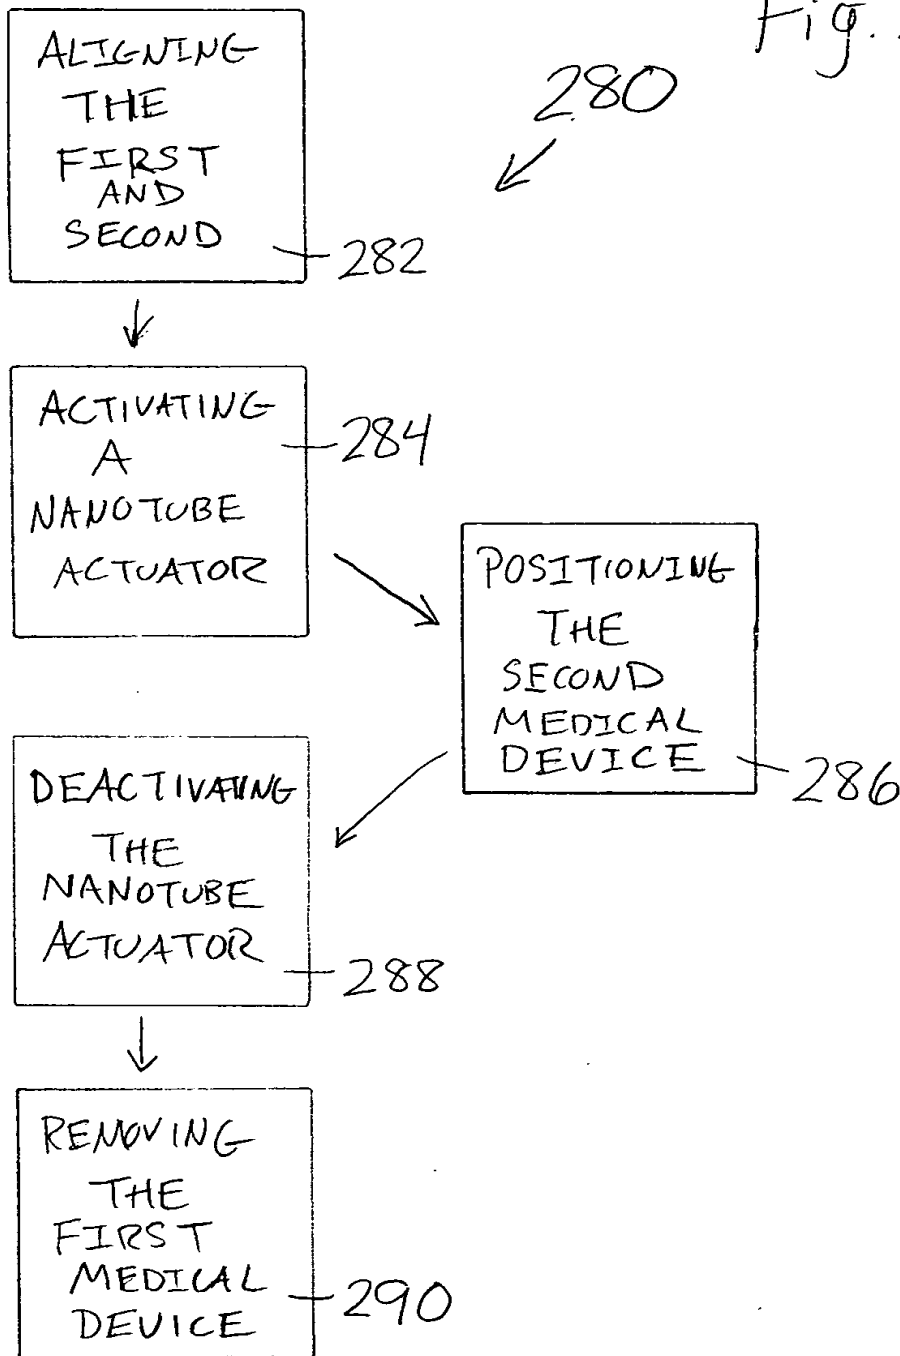


Fig. 20



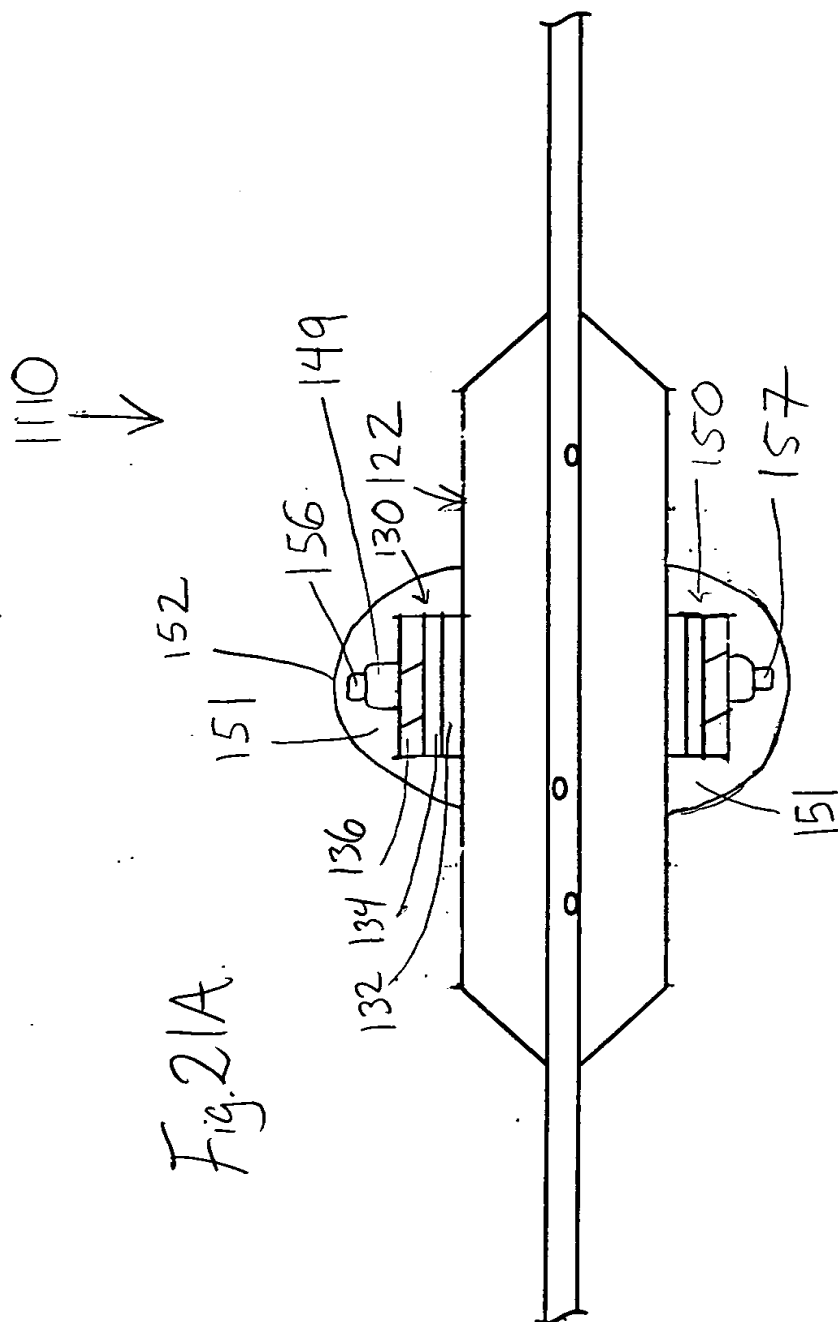


Fig. 21C



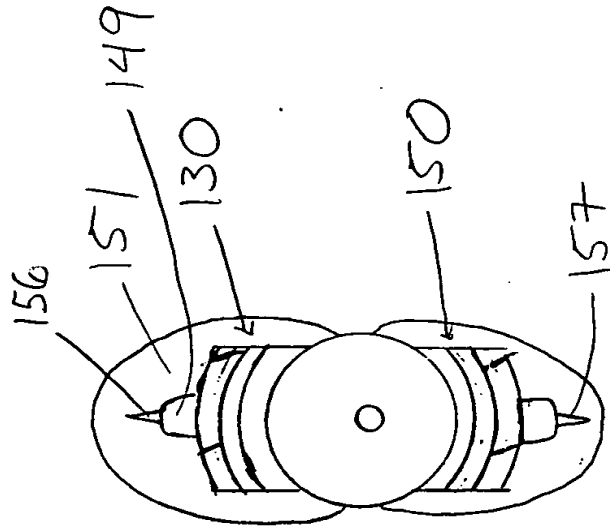


Fig. 21B

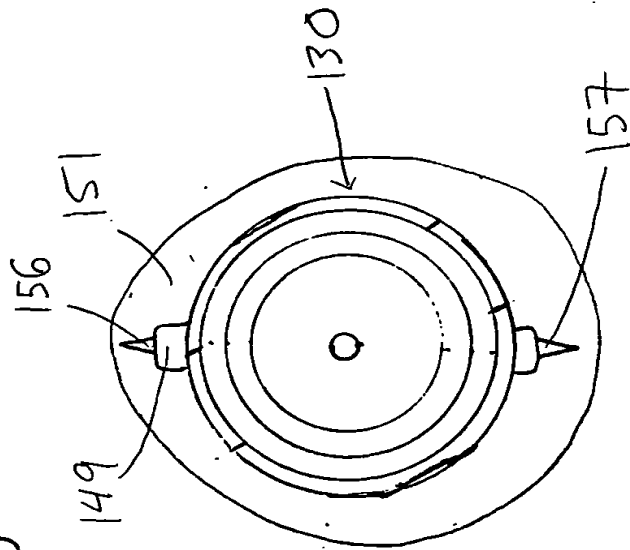

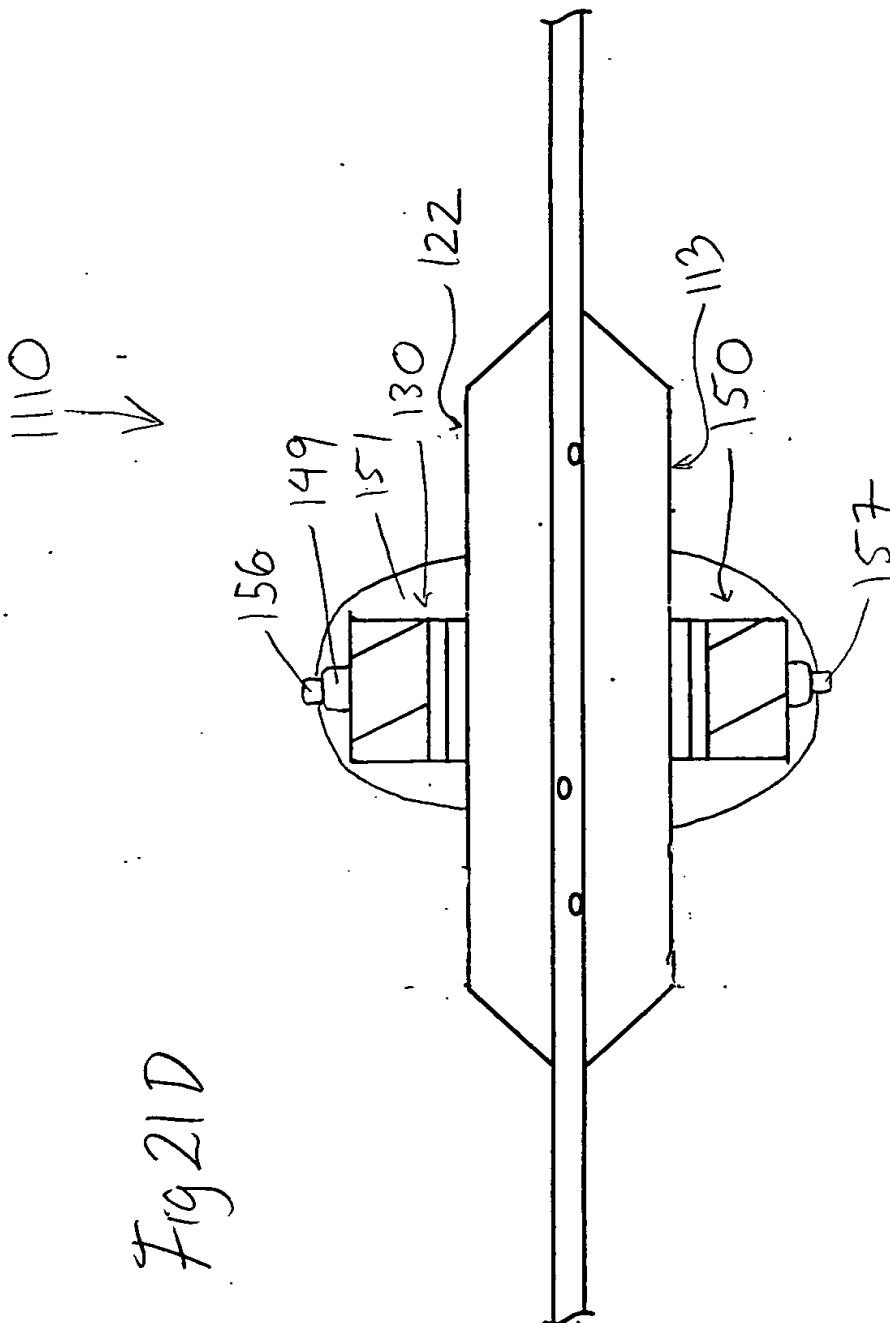

Atty Docket No. 29985/02-032I
Title: Nano-Actuated Medical Device
Inventor: Weber, et al.
Figures 21E and 21F
Sheet 25 of 45

Fig. 21F

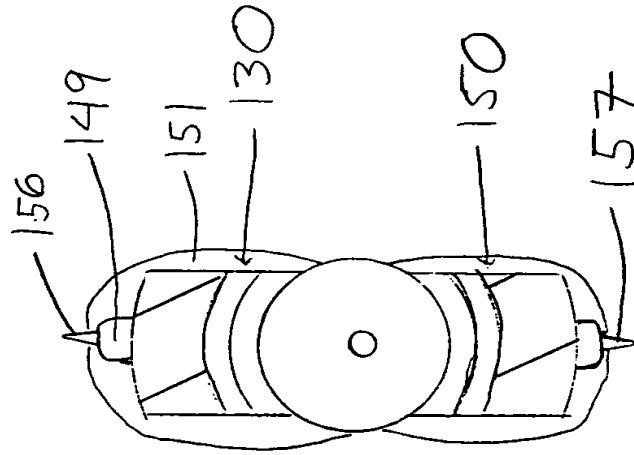
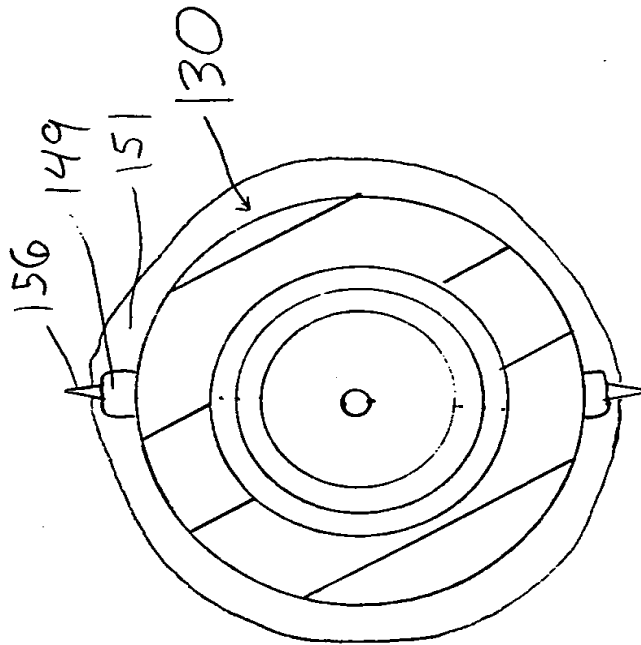


Fig. 21E




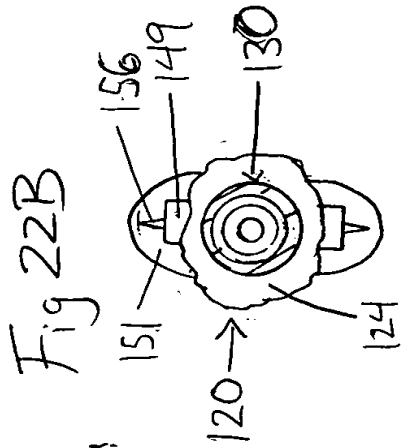


Fig 22A

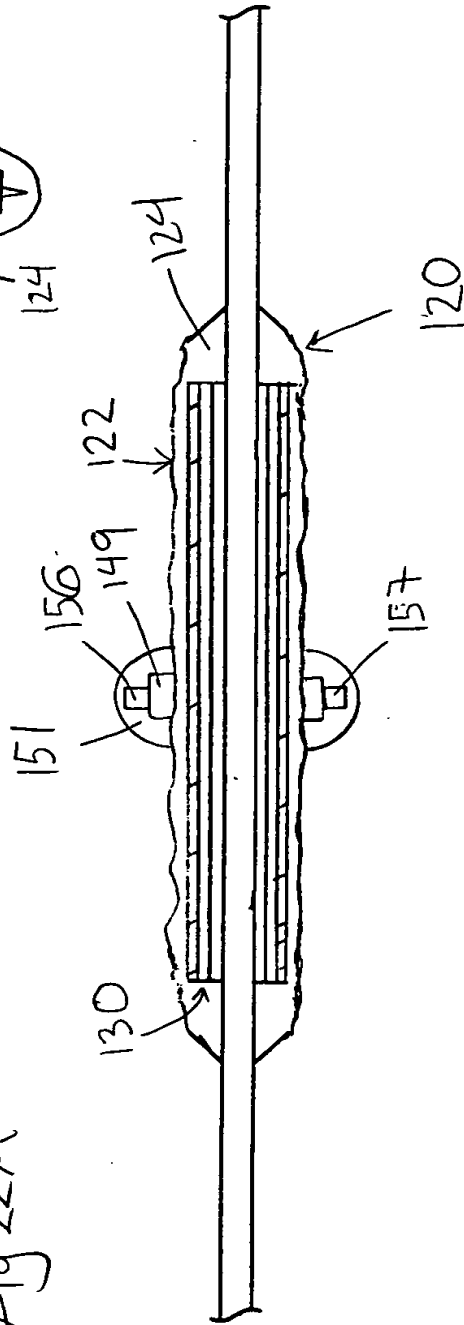

↑
1210

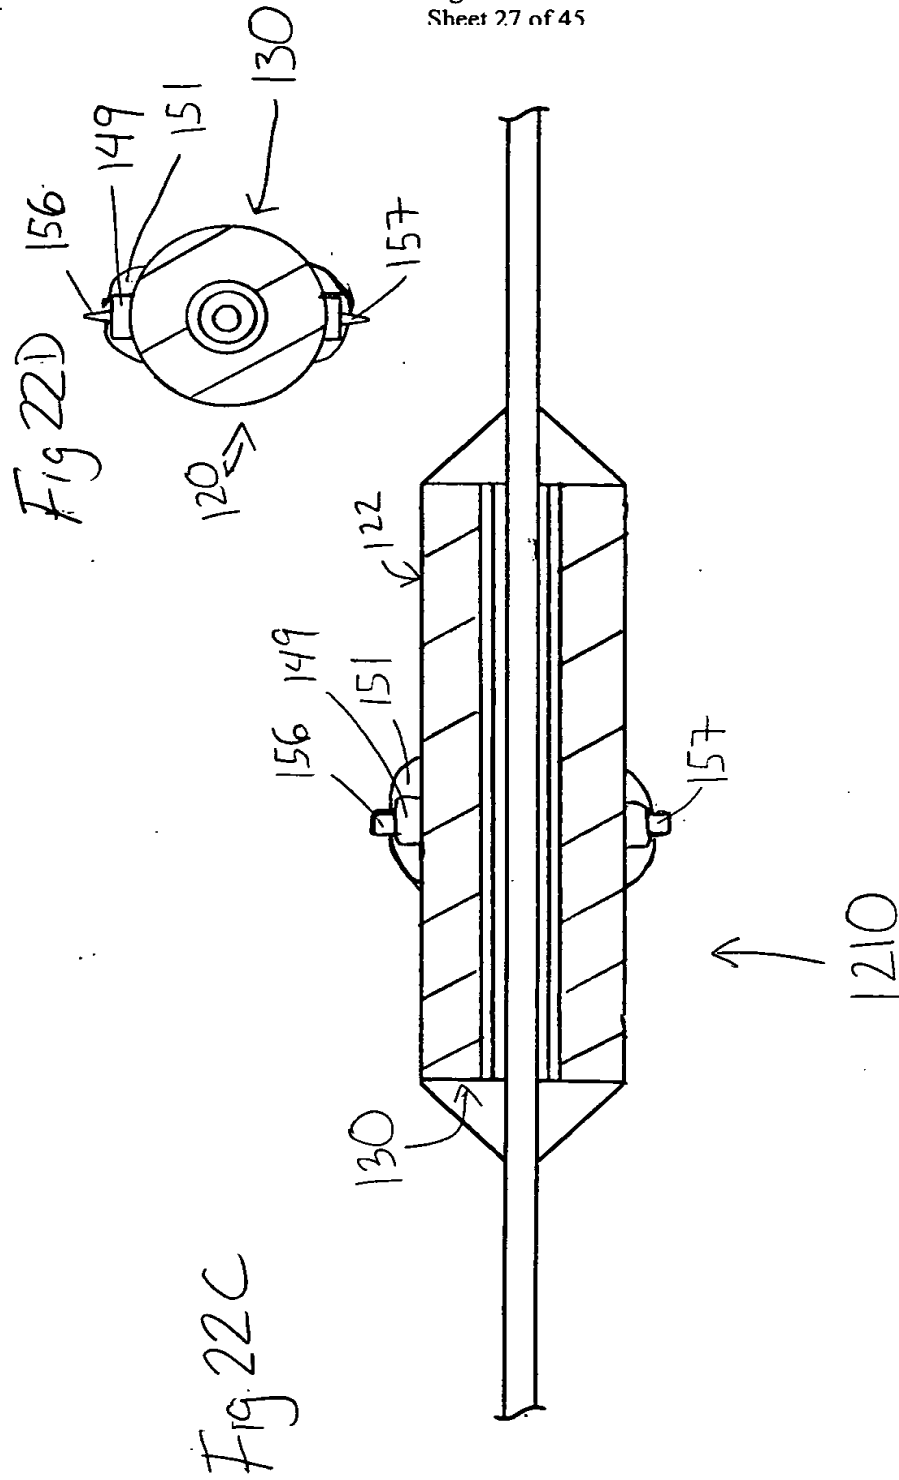


Fig 23

← 380

POSITIONING
THE
BLADE

382



ACTIVATING
THE
ACTUATOR

384




CUTTING
WITH
THE
BLADE

386



DEACTIVATING
THE
ACTUATOR

388



REMOVING
THE
MEDICAL
DEVICE

390

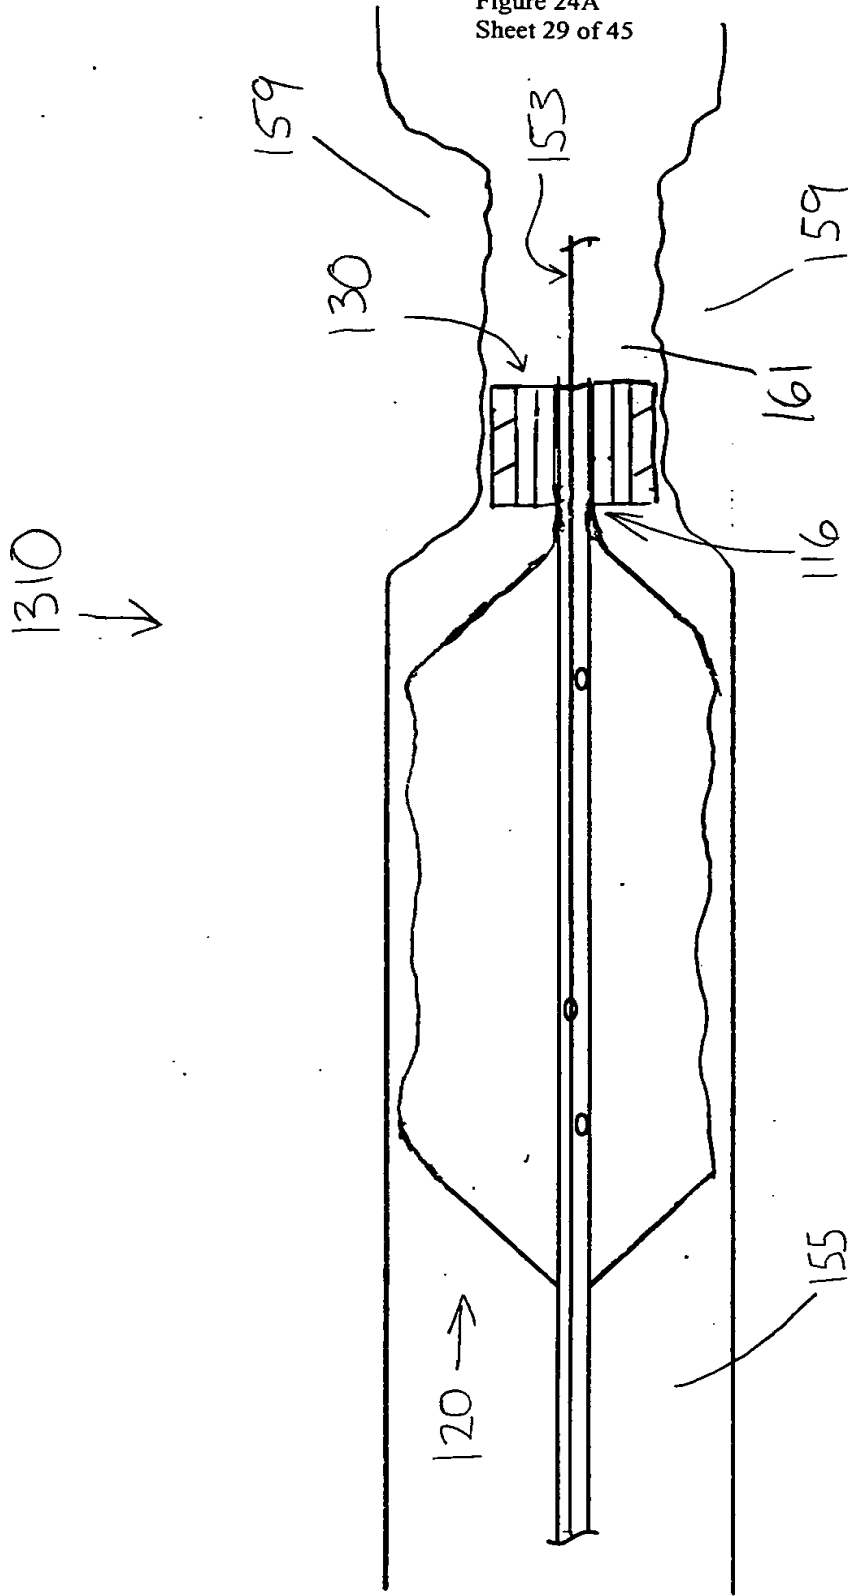


Fig. 24A

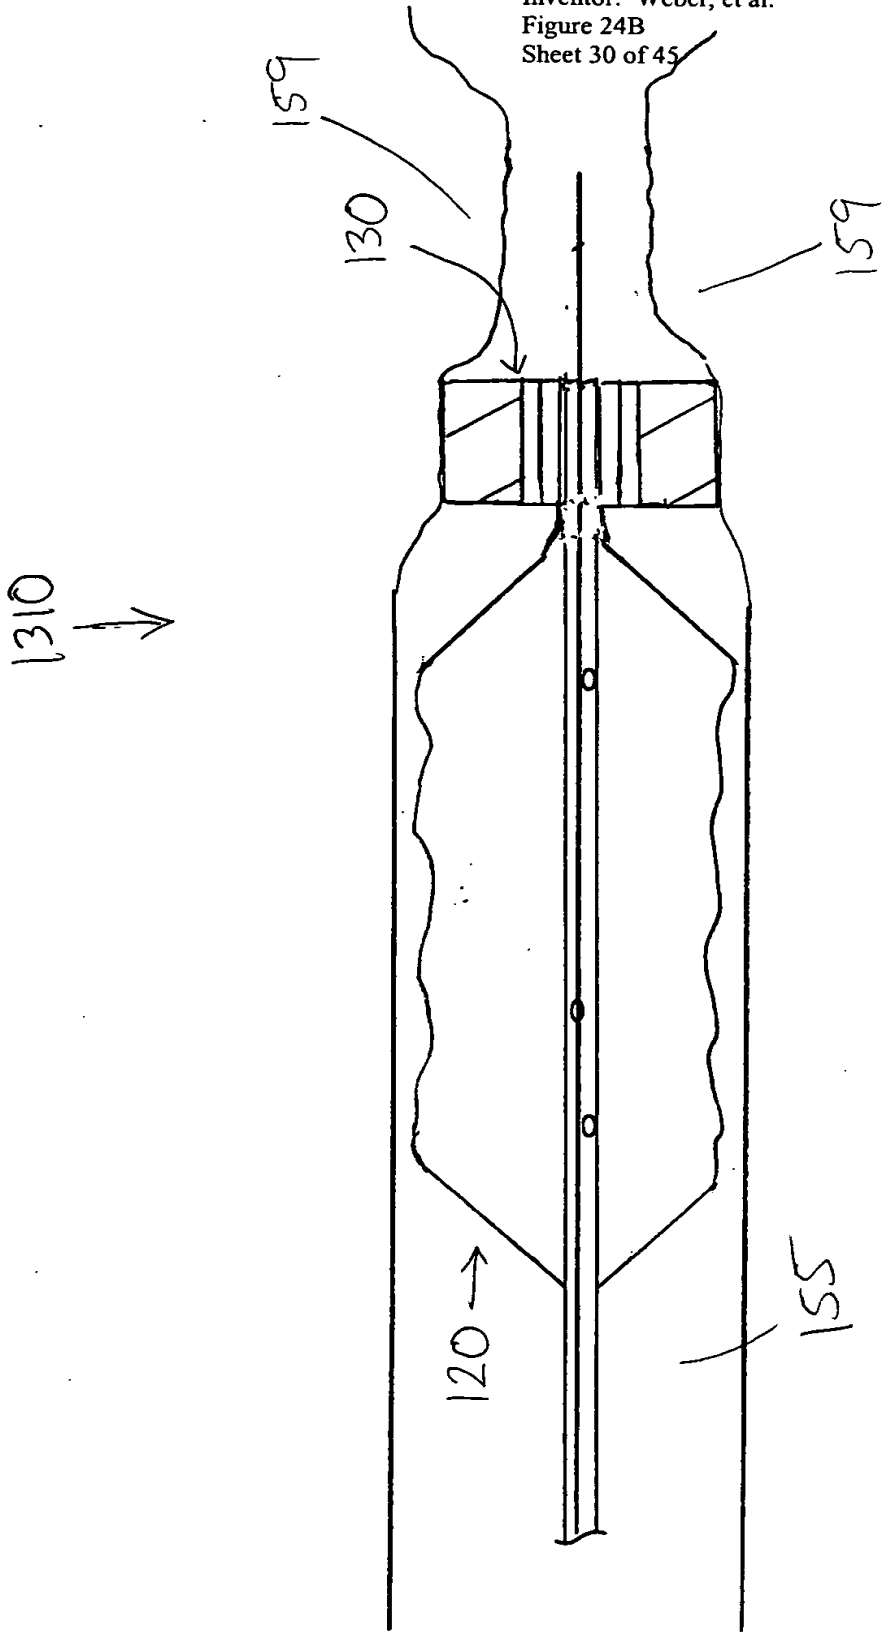


Fig 24B

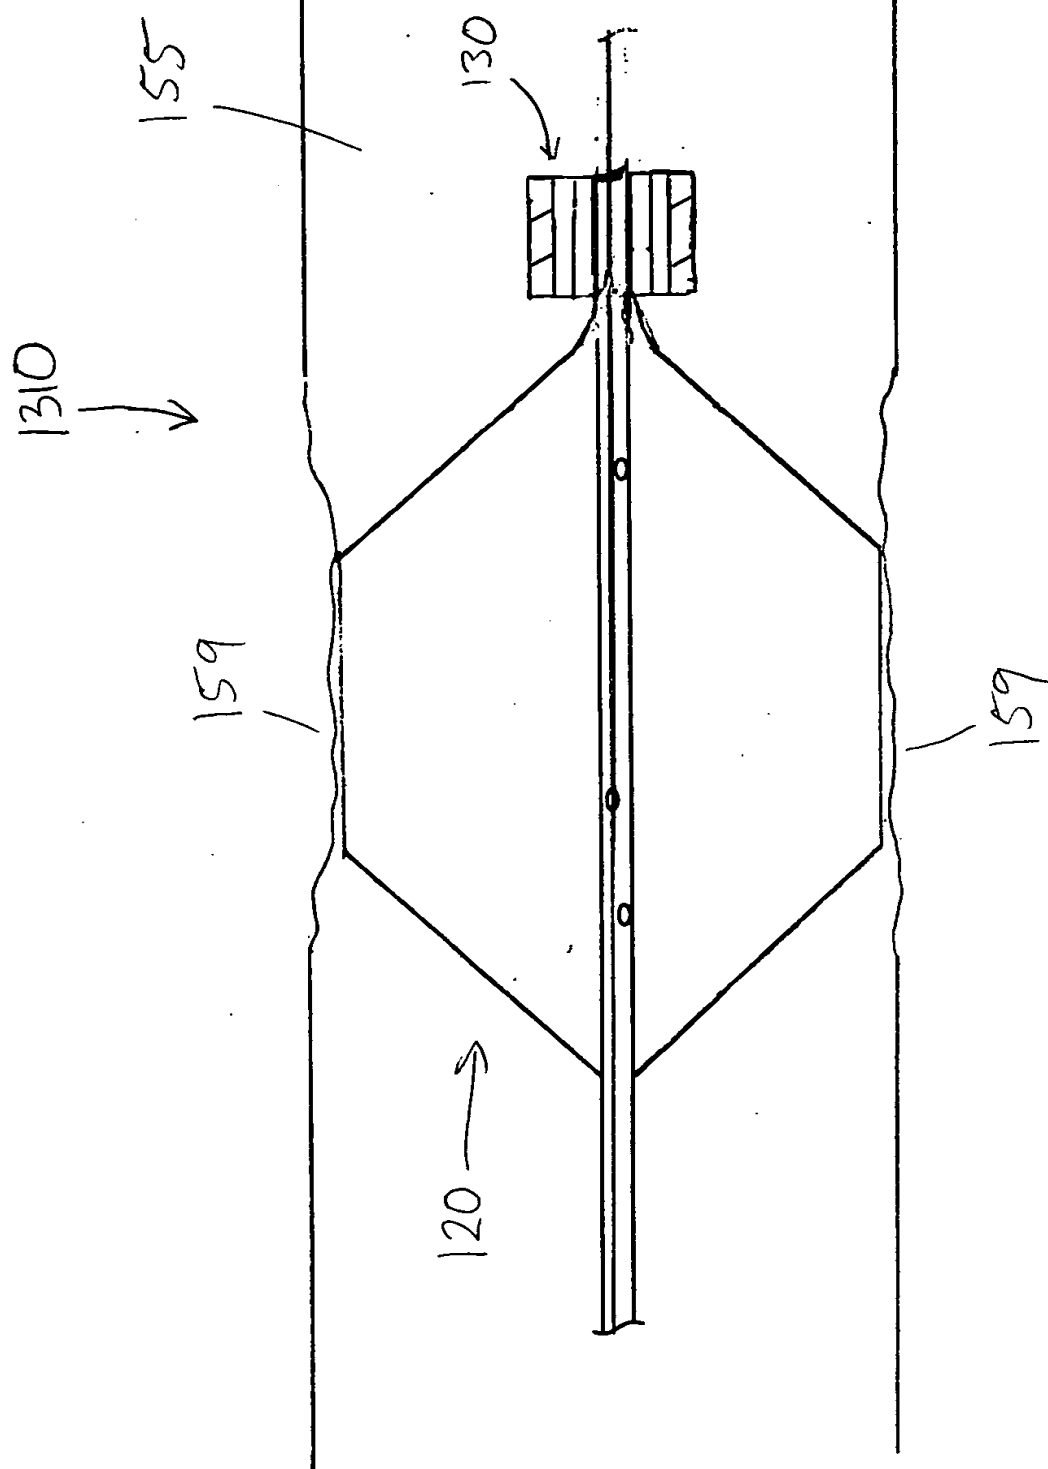


Fig. 24C

Fig. 25

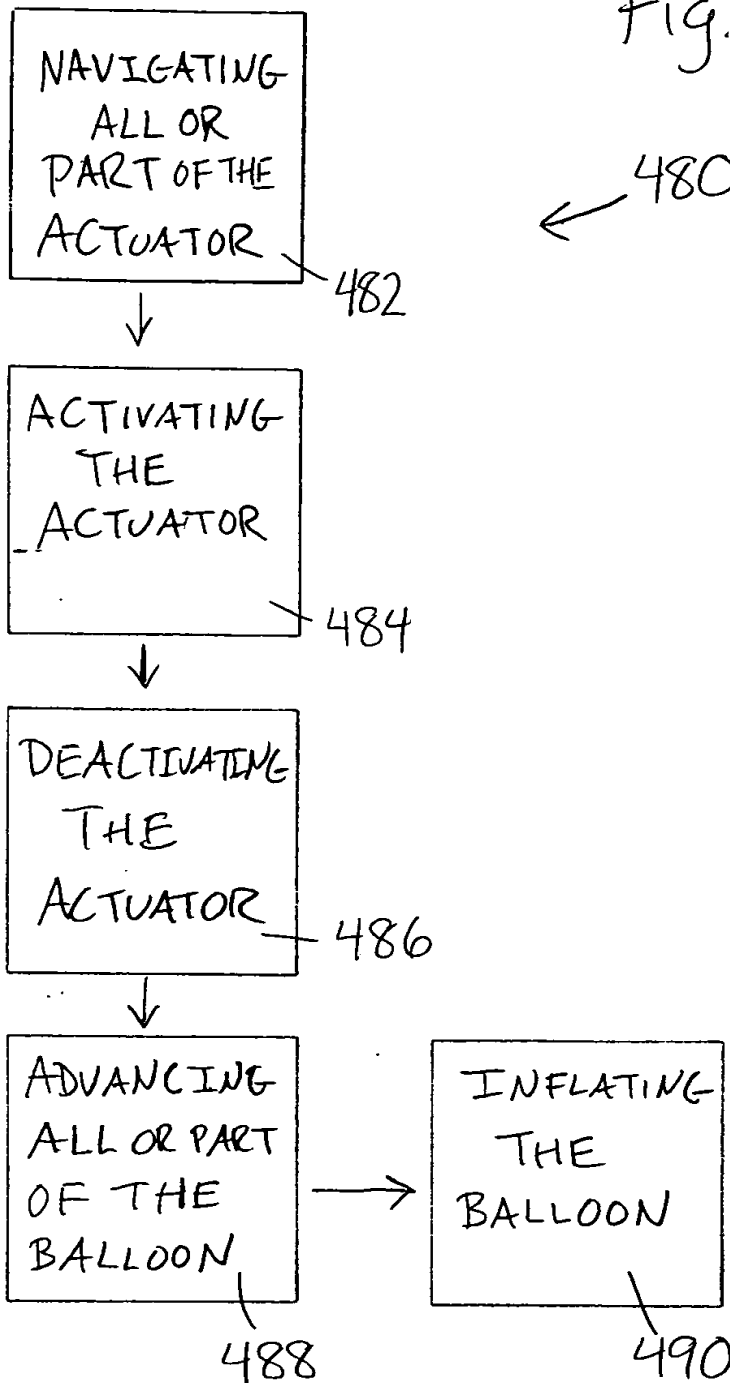


Fig. 26A

1410

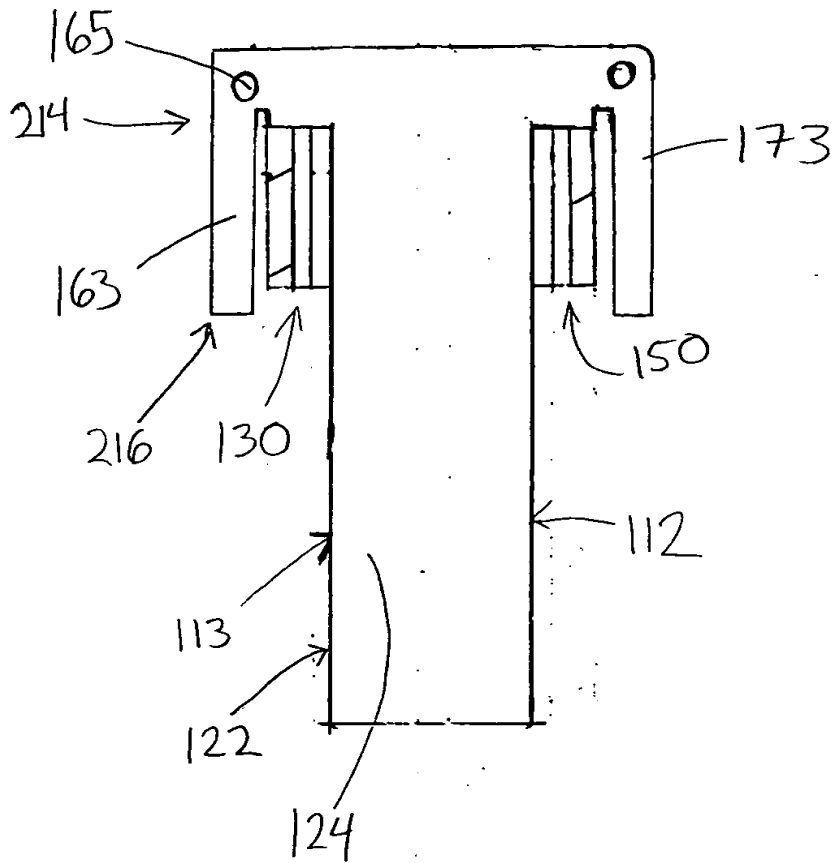


Fig 26B

1410

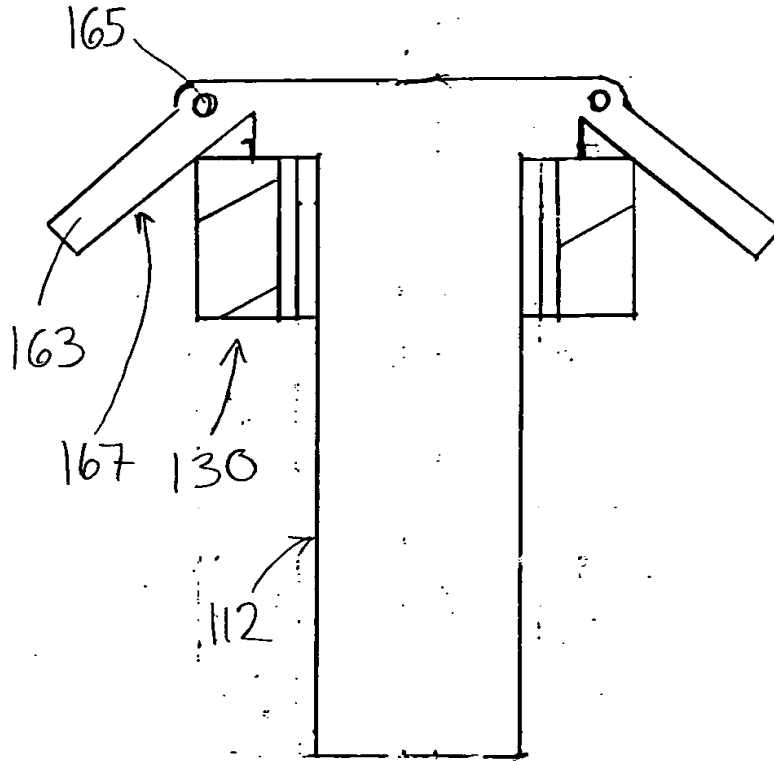


Fig. 27A

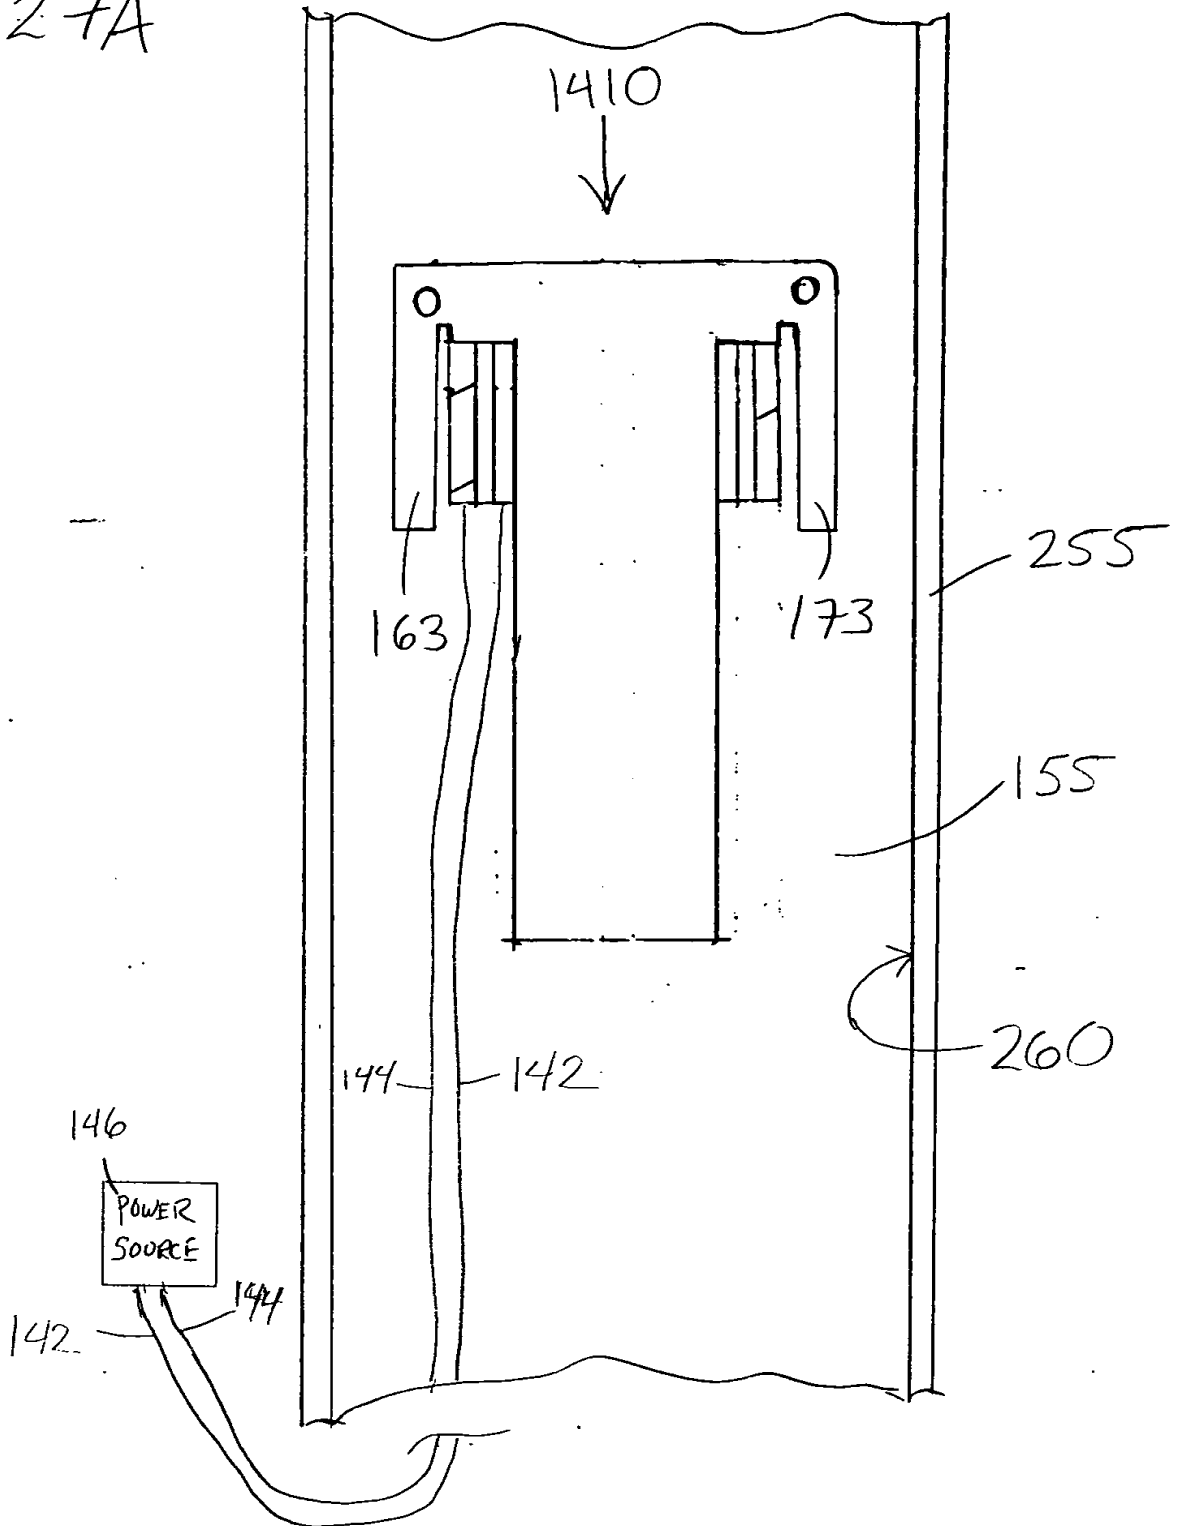


Fig. 27B

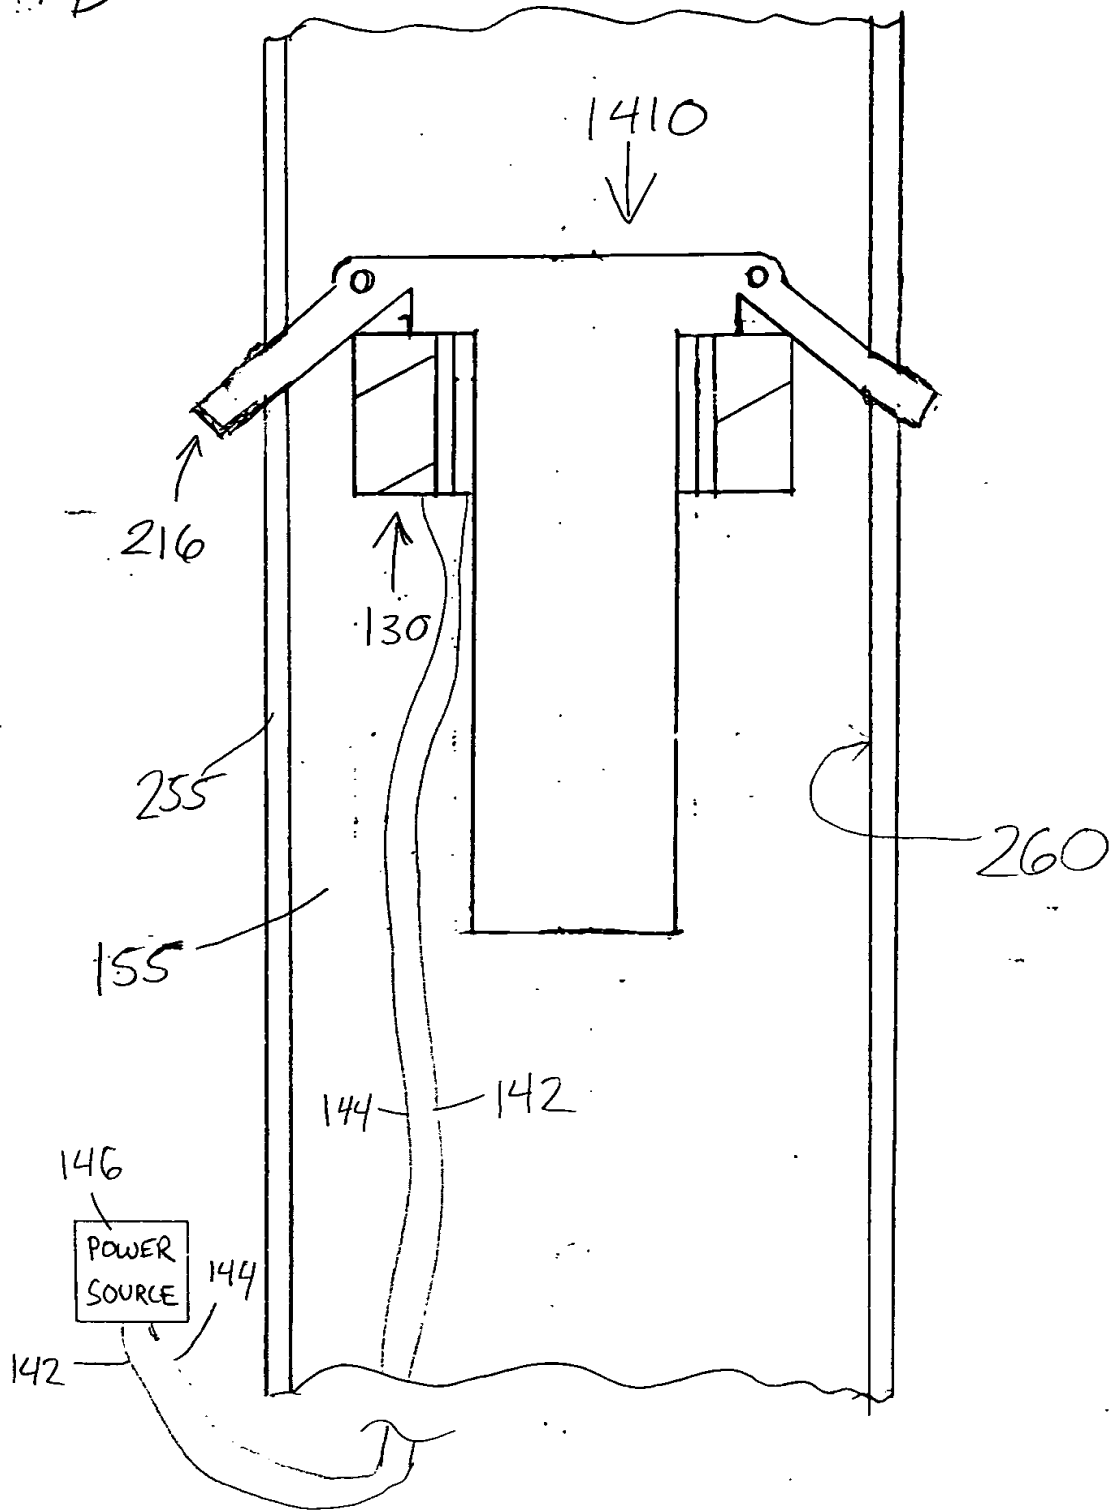


Fig. 28

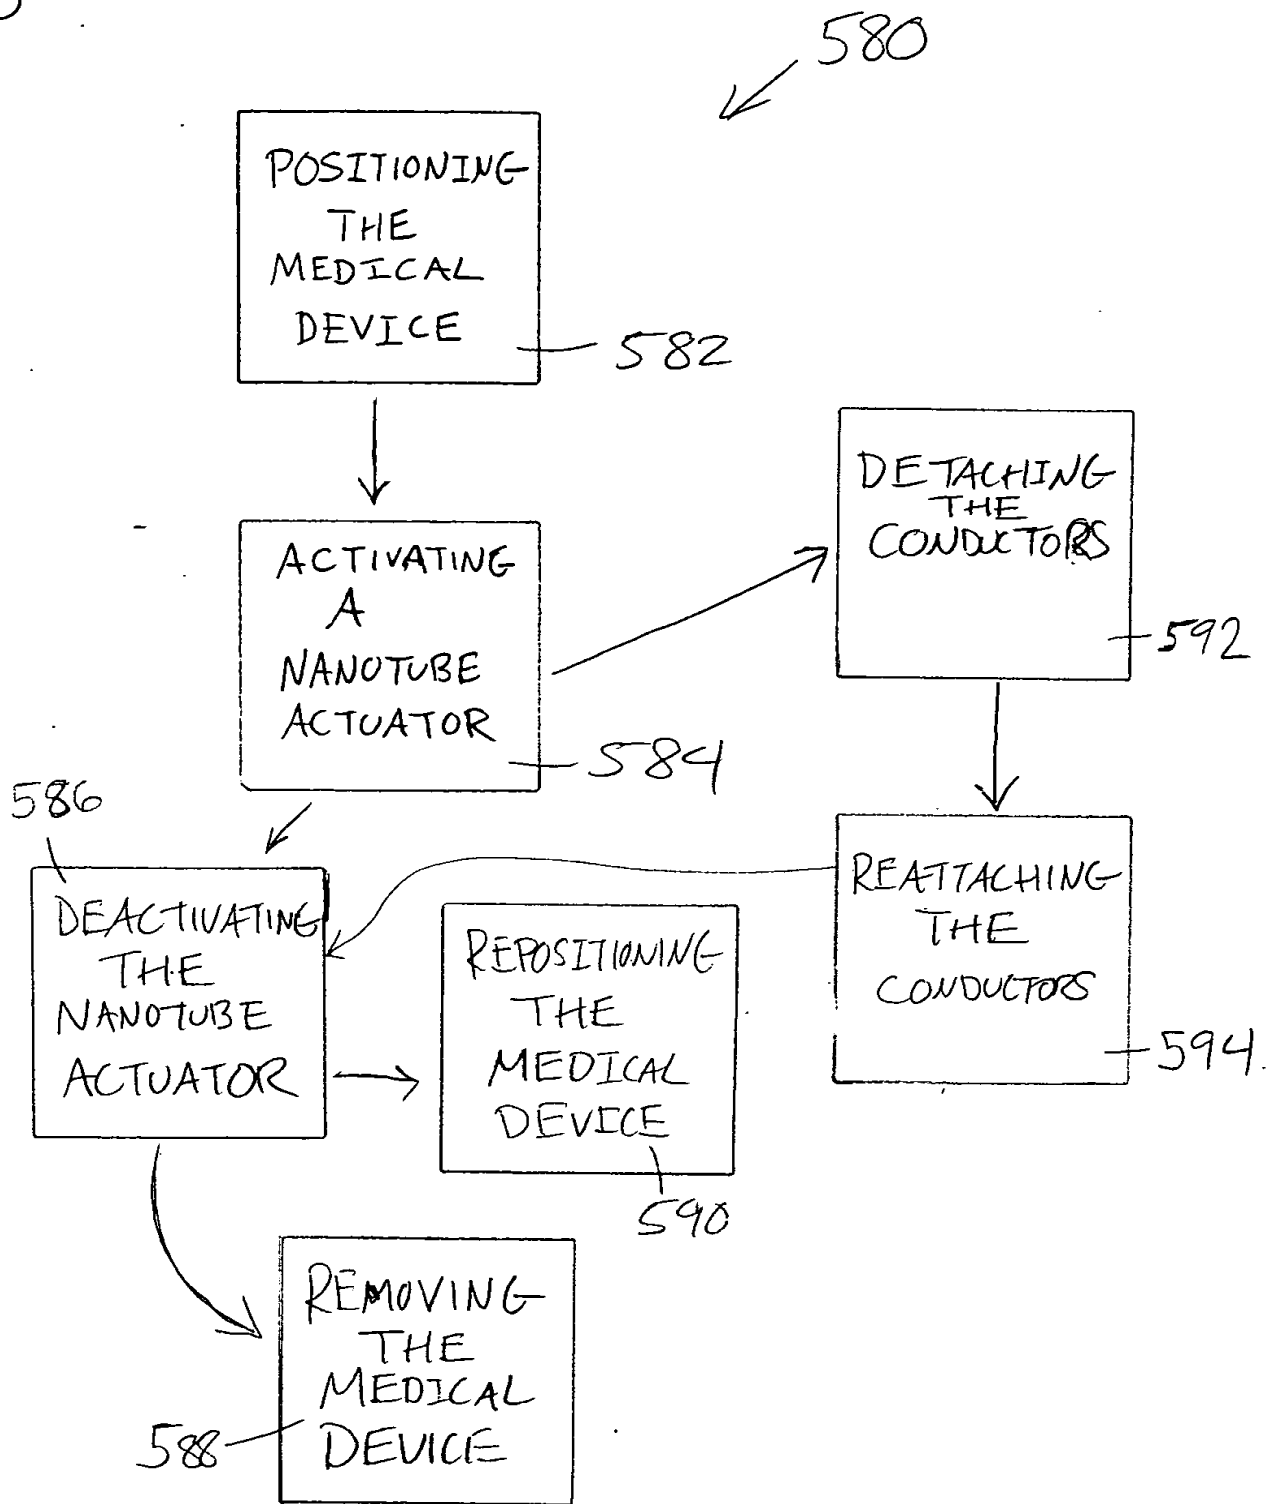


Fig. 29A

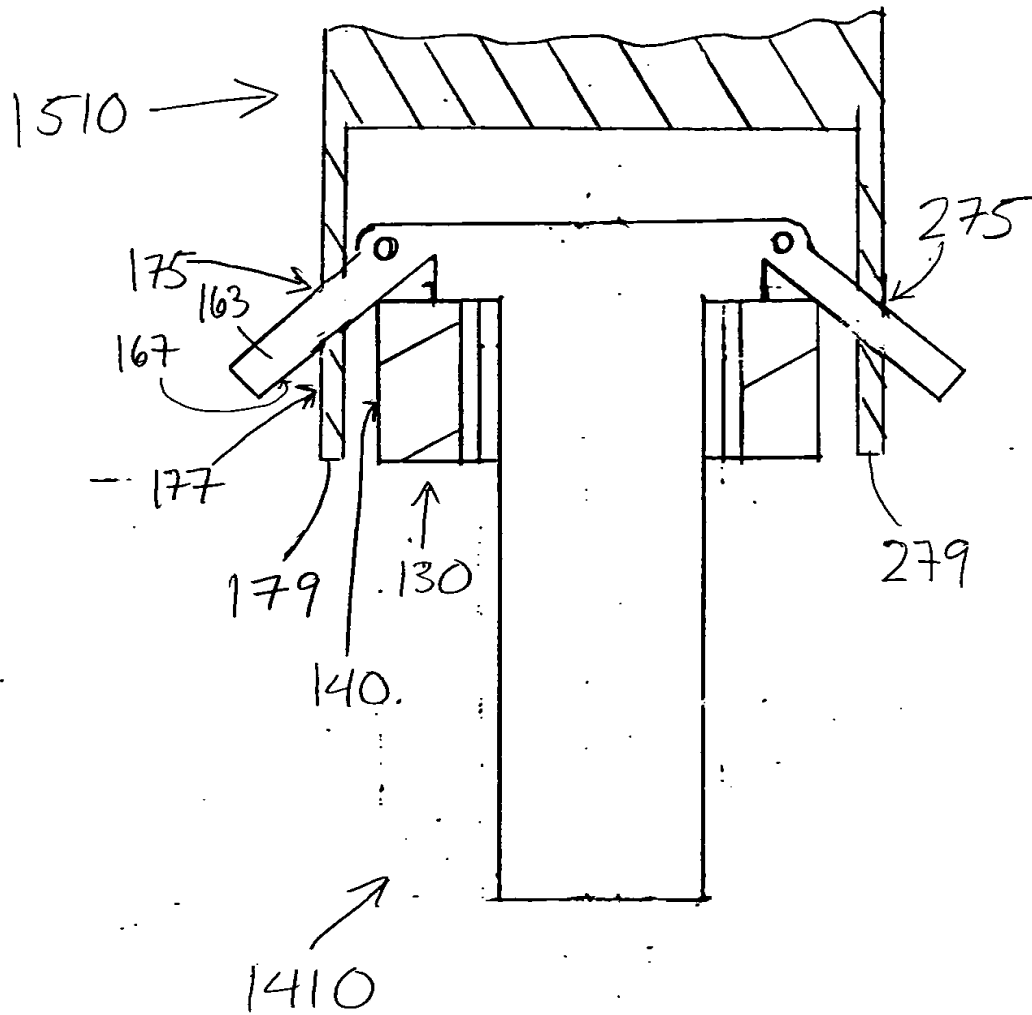
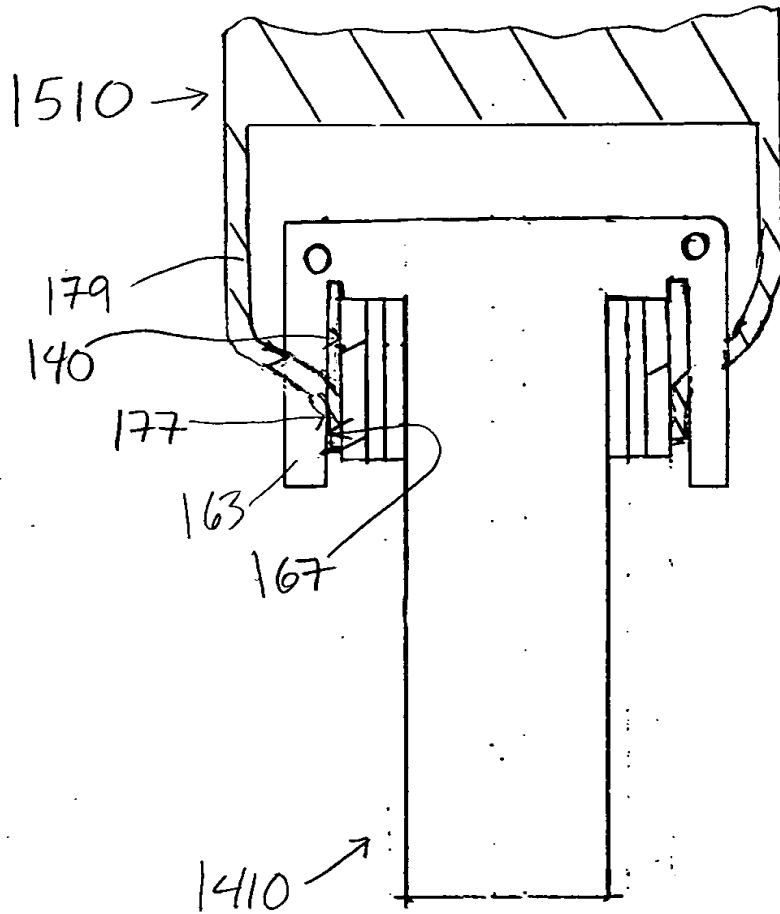
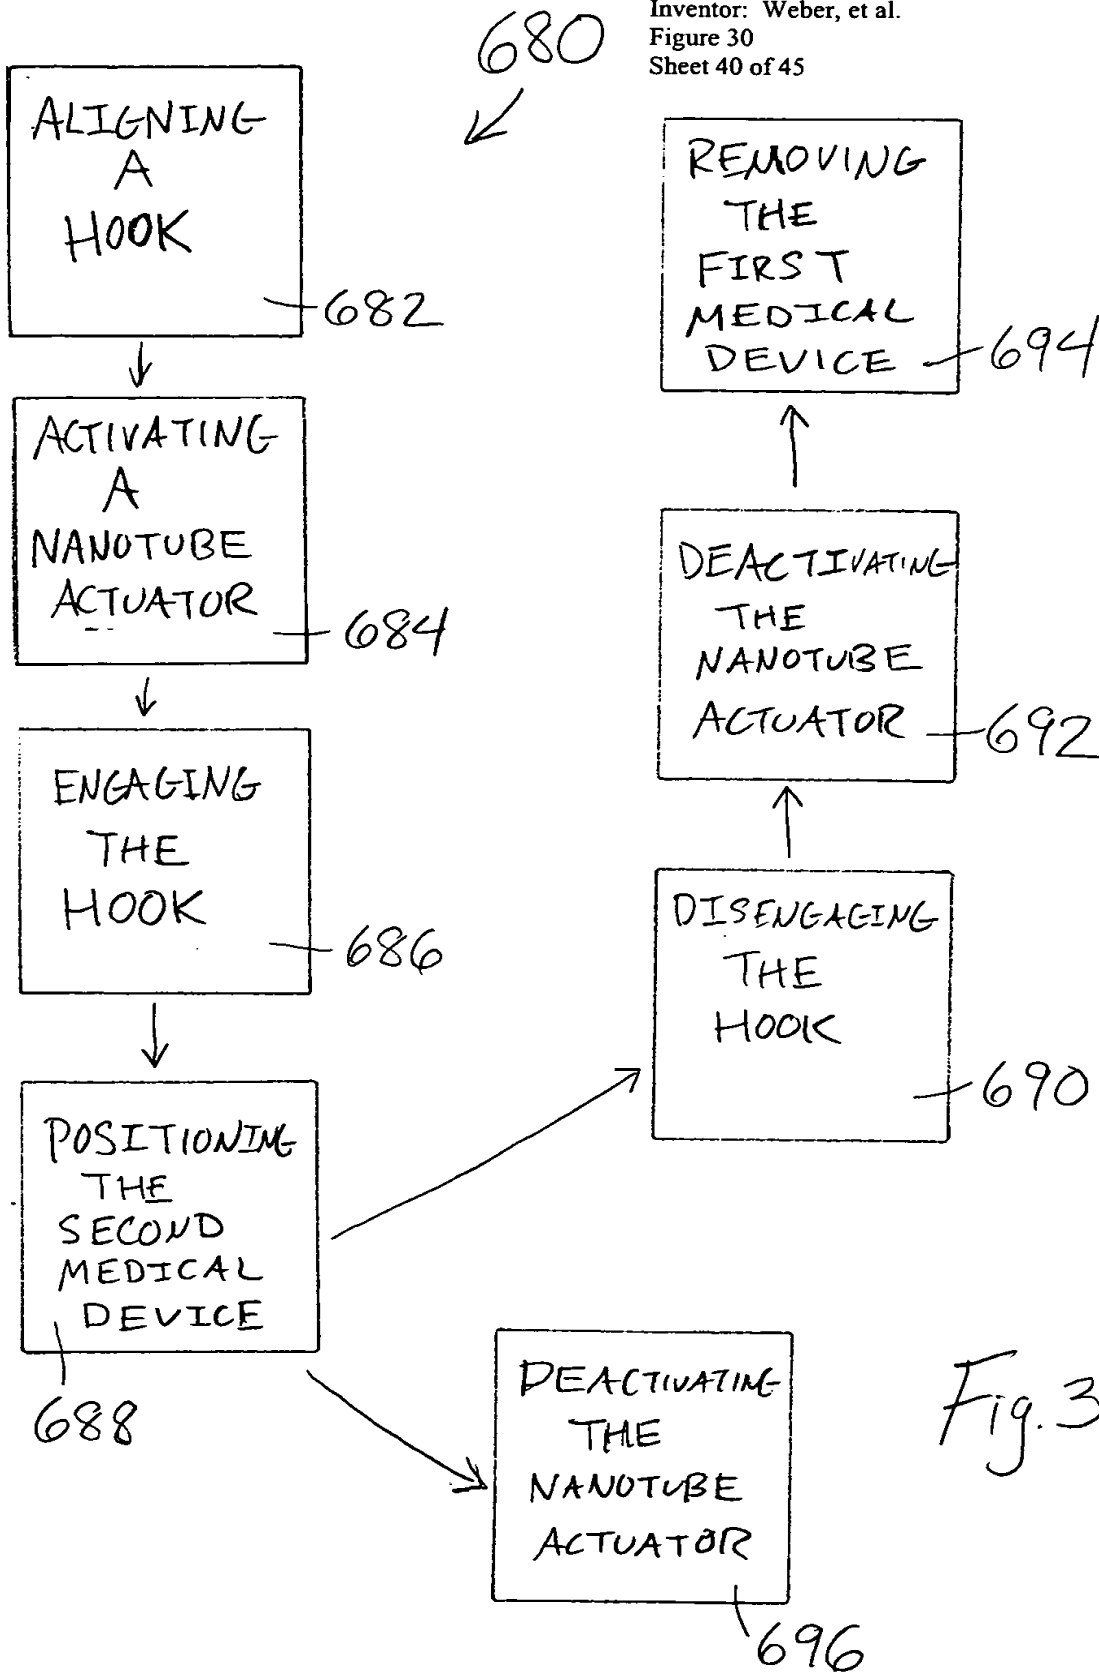
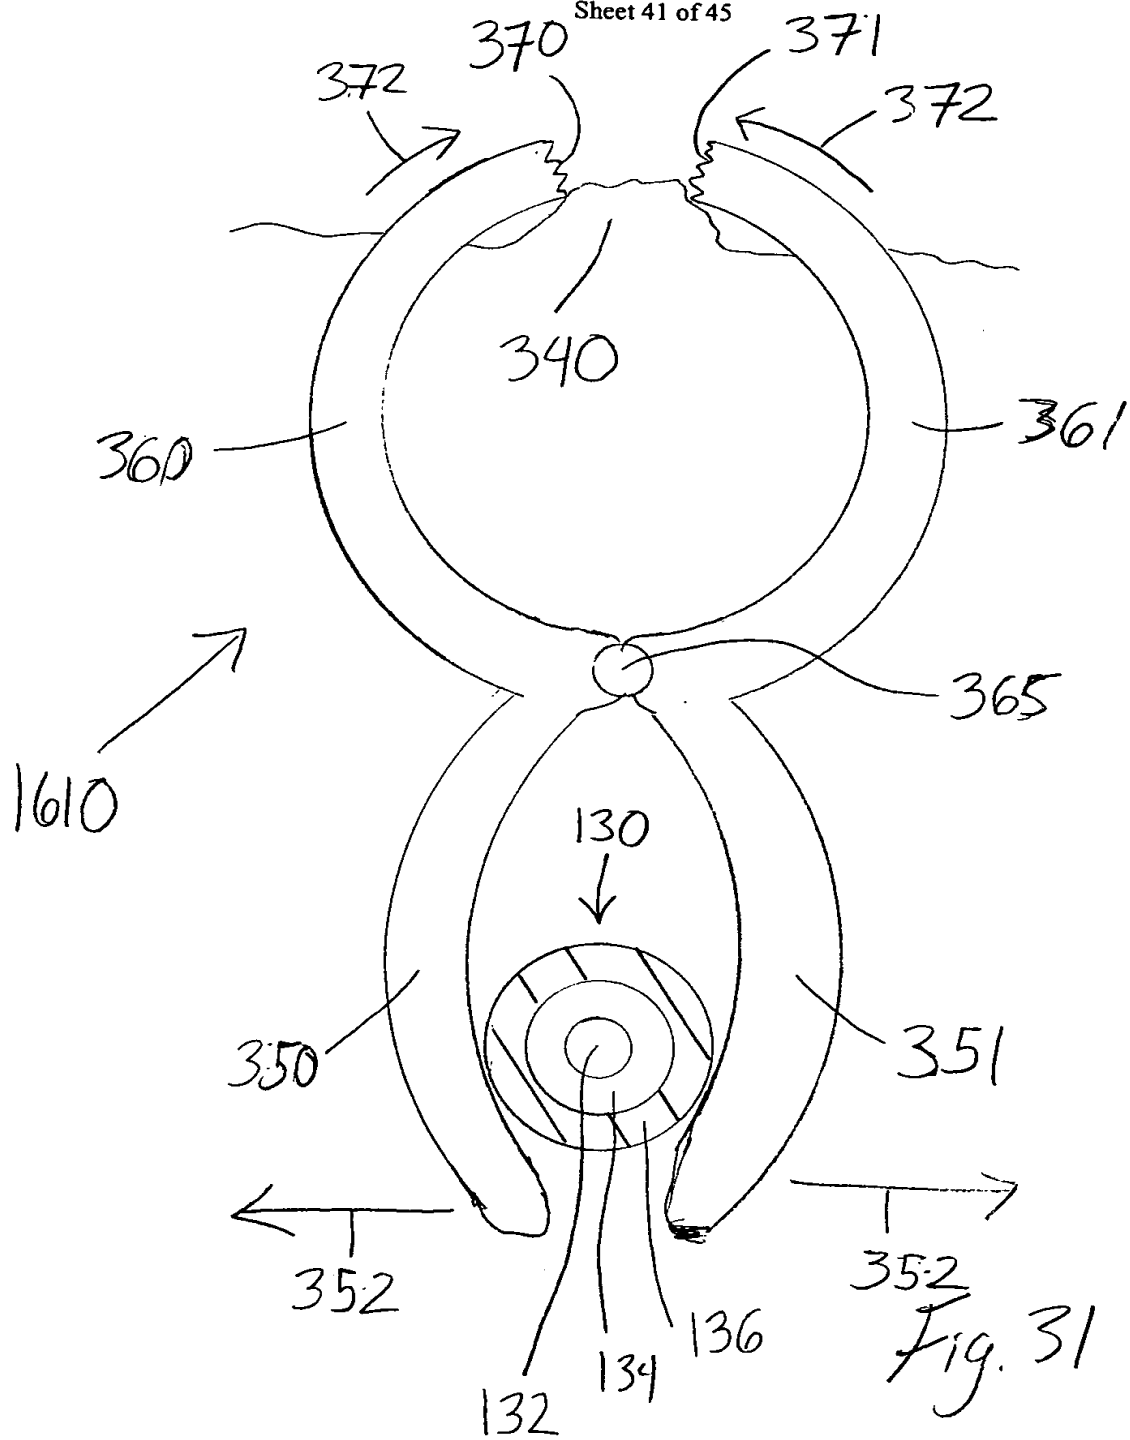



Fig. 29B

Atty Docket No. 29985/02-0321
Title: Nano-Actuated Medical Device
Inventor: Weber, et al.
Figure 29B
Sheet 39 of 45







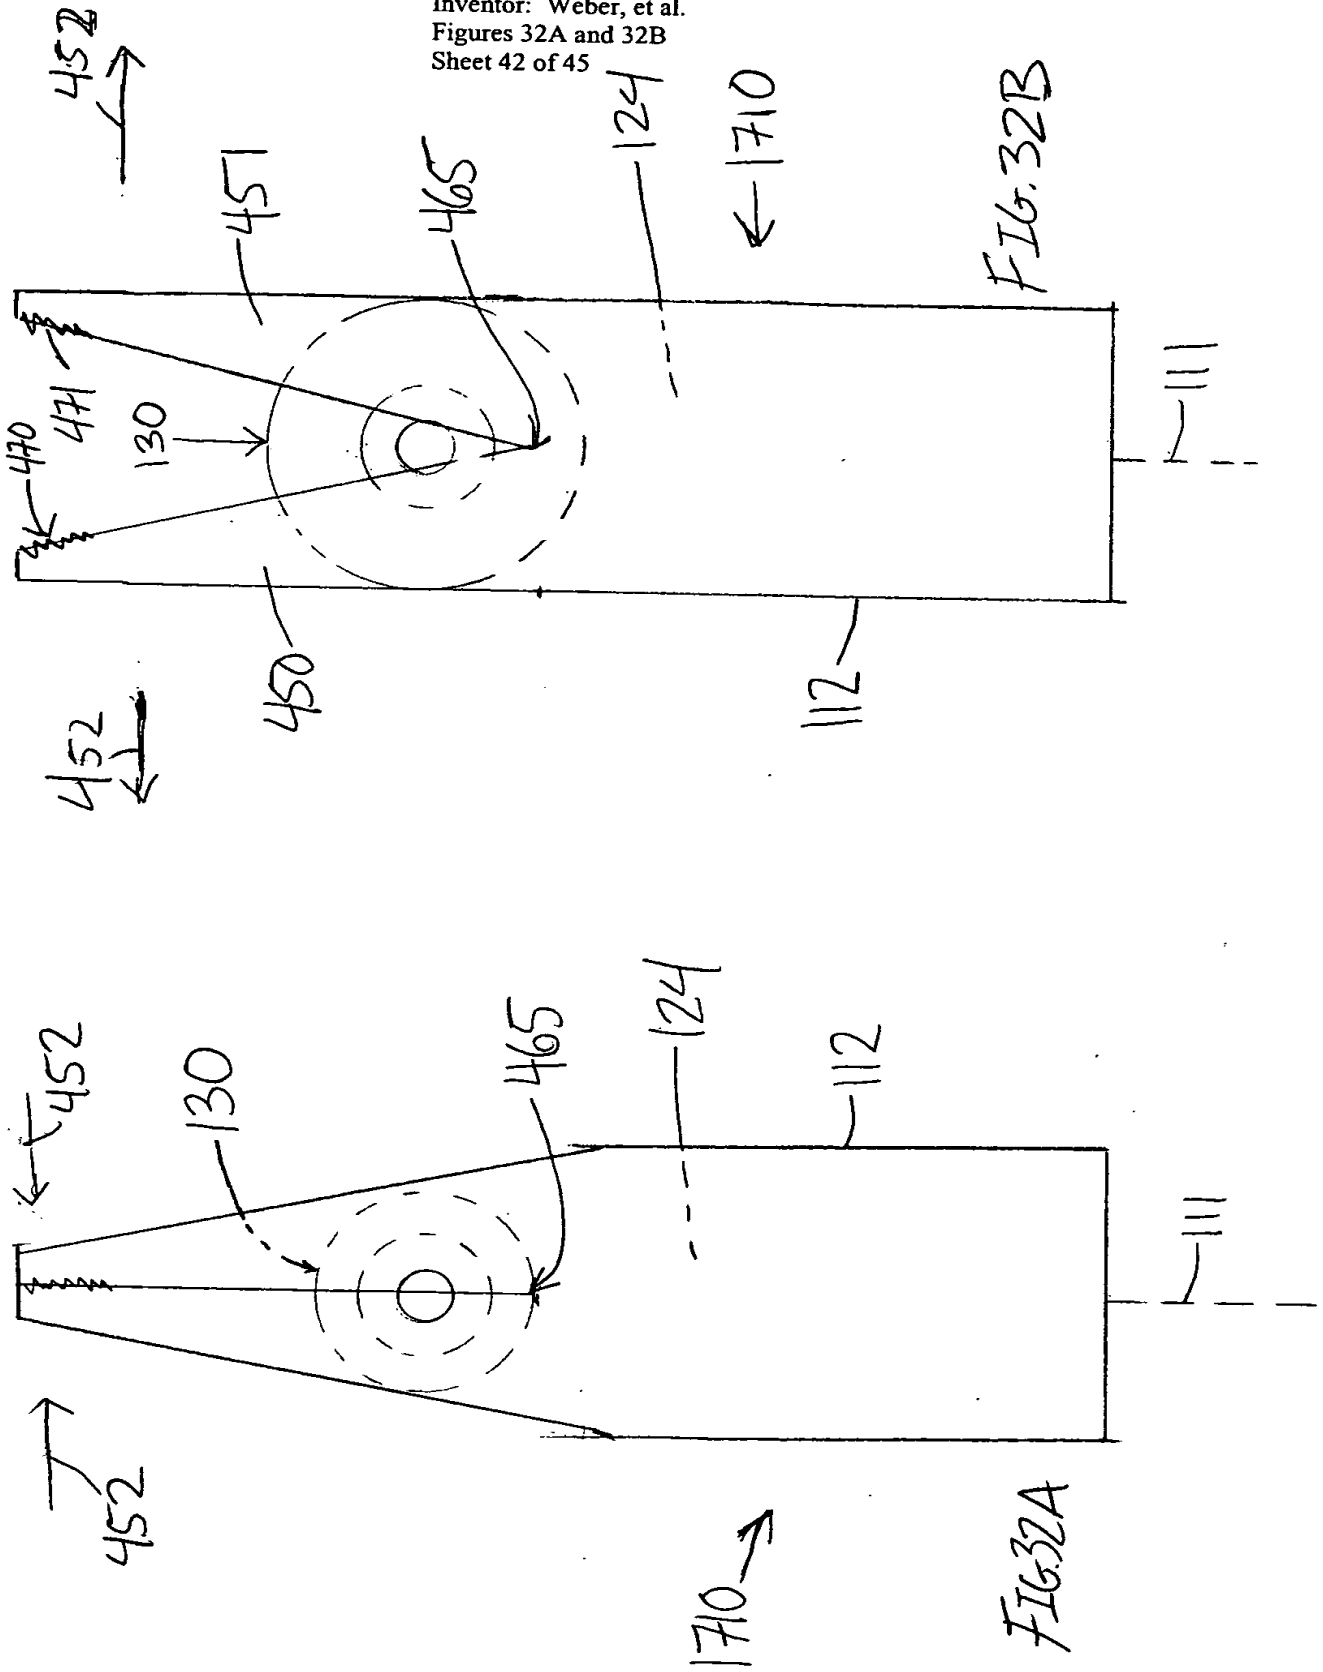

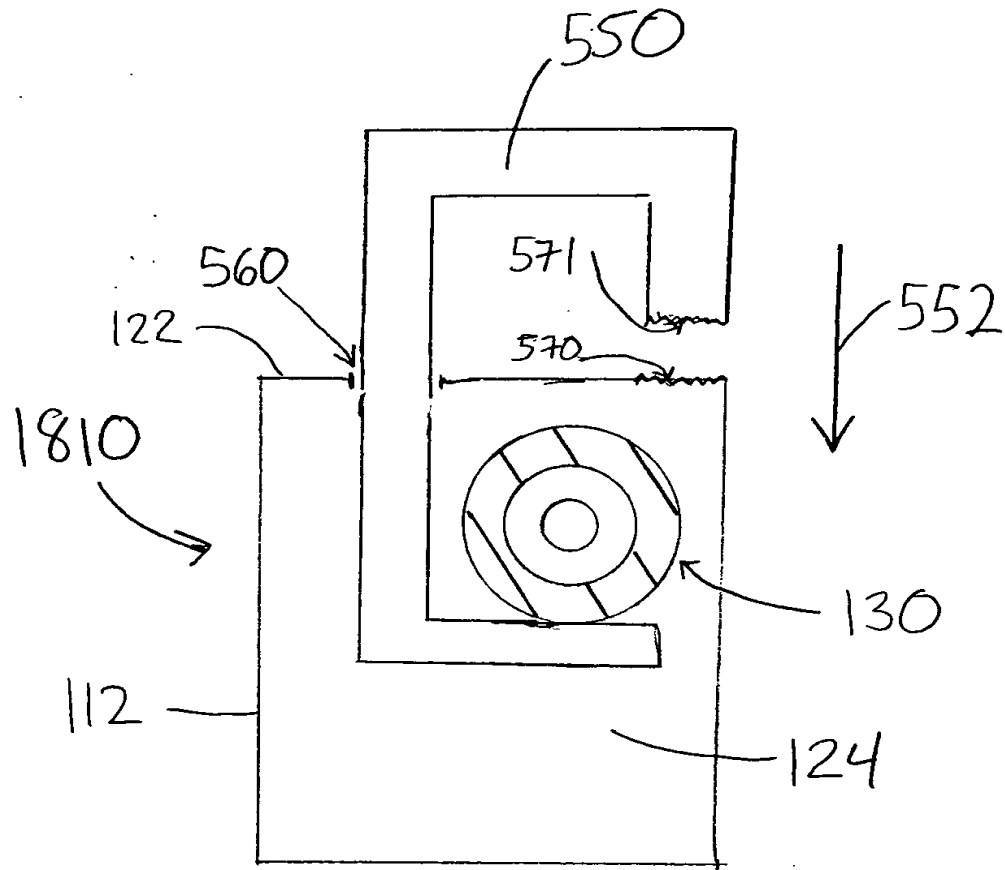


FIG. 33

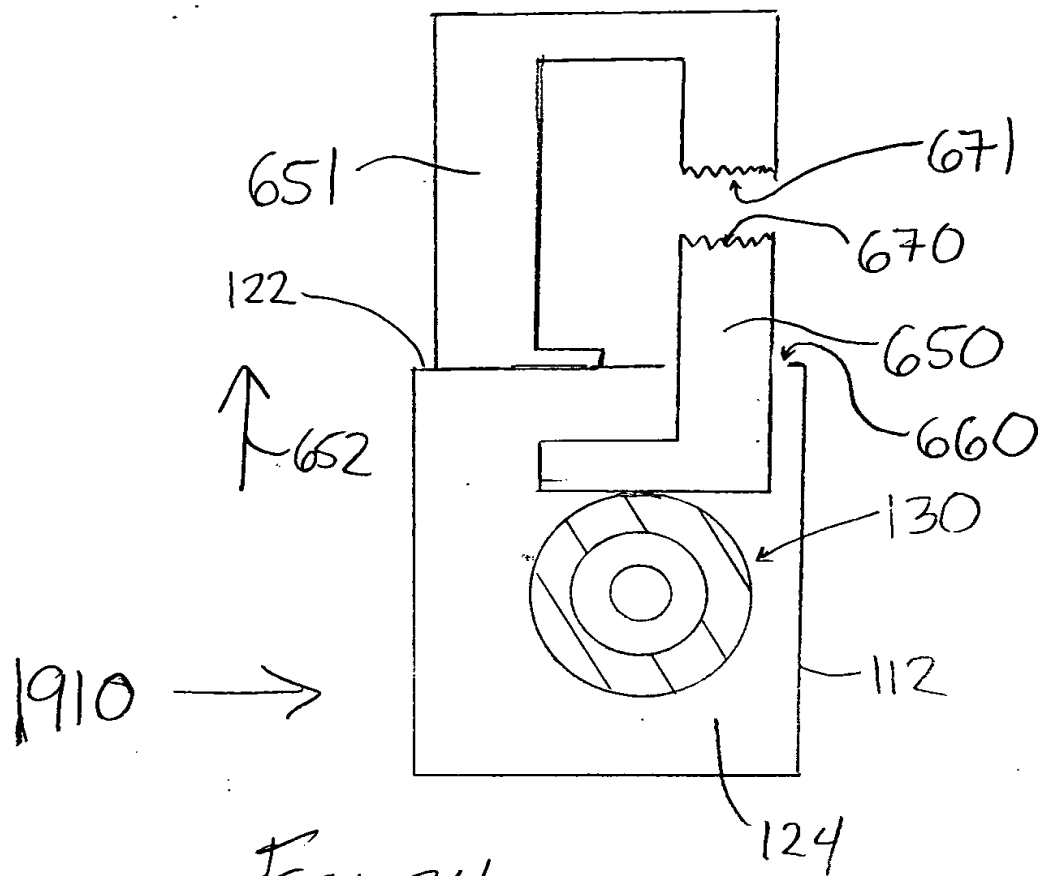


FIG. 35

